

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Cochrane COVID-19 Diagnostic Test Accuracy Group; Dinnes, Jacqueline; Deeks, Jon; Adriano, Ada; Berhane, Sarah; Davenport, Clare; Dittrich, Sabine ; Emperador, Devy ; Takwoingi, Yemisi; Cunningham, Jane ; Beese, Sophie; Dretzke, Janine; Ferrante di Ruffano, Lavinia; Harris, Isobel ; Price, Malcolm; Taylor-Phillips, Sian; Hooft, Lotty; Leeflang, Mariska M G; Spijker, René ; Van De Bruel, Ann

DOI:

DOI: [10.1002/14651858.CD013705](https://doi.org/10.1002/14651858.CD013705).

License:

Creative Commons: Attribution-NonCommercial (CC BY-NC)

Document Version

Publisher's PDF, also known as Version of record

Citation for published version (Harvard):

Cochrane COVID-19 Diagnostic Test Accuracy Group, Dinnes, J, Deeks, J, Adriano, A, Berhane, S, Davenport, C, Dittrich, S, Emperador, D, Takwoingi, Y, Cunningham, J, Beese, S, Dretzke, J, Ferrante di Ruffano, L, Harris, I, Price, M, Taylor-Phillips, S, Hooft, L, Leeflang, MMG, Spijker, R & Van De Bruel, A 2020, 'Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)', *Cochrane Database of Systematic Reviews*, no. 8, CD013705. <https://doi.org/DOI: 10.1002/14651858.CD013705>.

[Link to publication on Research at Birmingham portal](#)

General rights

Unless a licence is specified above, all rights (including copyright and moral rights) in this document are retained by the authors and/or the copyright holders. The express permission of the copyright holder must be obtained for any use of this material other than for purposes permitted by law.

- Users may freely distribute the URL that is used to identify this publication.
- Users may download and/or print one copy of the publication from the University of Birmingham research portal for the purpose of private study or non-commercial research.
- User may use extracts from the document in line with the concept of 'fair dealing' under the Copyright, Designs and Patents Act 1988 (?)
- Users may not further distribute the material nor use it for the purposes of commercial gain.

Where a licence is displayed above, please note the terms and conditions of the licence govern your use of this document.

When citing, please reference the published version.

Take down policy

While the University of Birmingham exercises care and attention in making items available there are rare occasions when an item has been uploaded in error or has been deemed to be commercially or otherwise sensitive.

If you believe that this is the case for this document, please contact UBIRA@lists.bham.ac.uk providing details and we will remove access to the work immediately and investigate.

Download date: 11. Jul. 2025



**Cochrane
Library**

Cochrane Database of Systematic Reviews

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Dinnes J, Deeks JJ, Adriano A, Berhane S, Davenport C, Dittrich S, Emperador D, Takwoingi Y, Cunningham J, Beese S, Dretzke J, Ferrante di Ruffano L, Harris IM, Price MJ, Taylor-Phillips S, Hooft L, Leeftang MMG, Spijker R, Van den Bruel A, Cochrane COVID-19 Diagnostic Test Accuracy Group

Dinnes J, Deeks JJ, Adriano A, Berhane S, Davenport C, Dittrich S, Emperador D, Takwoingi Y, Cunningham J, Beese S, Dretzke J, Ferrante di Ruffano L, Harris IM, Price MJ, Taylor-Phillips S, Hooft L, Leeftang MMG, Spijker R, Van den Bruel A.

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection.

Cochrane Database of Systematic Reviews 2020, Issue 8. Art. No.: CD013705.

DOI: [10.1002/14651858.CD013705](https://doi.org/10.1002/14651858.CD013705).

www.cochranelibrary.com

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

WILEY

TABLE OF CONTENTS

HEADER	1
ABSTRACT	1
PLAIN LANGUAGE SUMMARY	3
SUMMARY OF FINDINGS	5
BACKGROUND	8
OBJECTIVES	10
METHODS	10
RESULTS	12
Figure 1.	13
Figure 2.	15
Figure 3.	17
Figure 4.	17
Figure 5.	18
Figure 6.	18
Figure 7.	19
DISCUSSION	20
AUTHORS' CONCLUSIONS	22
ACKNOWLEDGEMENTS	23
REFERENCES	24
CHARACTERISTICS OF STUDIES	30
DATA	94
Test 1. Antigen tests - All	95
Test 2. Antigen tests - high viral load	95
Test 3. Antigen tests - low viral load	95
Test 4. Molecular tests - all	96
Test 5. Molecular tests - all (before discrepant analysis)	96
Test 6. Molecular tests - all (after discrepant analysis)	96
Test 7. Molecular tests - high viral load	96
Test 8. Molecular tests - low viral load	97
ADDITIONAL TABLES	97
APPENDICES	105
Figure 8.	128
HISTORY	129
CONTRIBUTIONS OF AUTHORS	129
DECLARATIONS OF INTEREST	130
SOURCES OF SUPPORT	130
DIFFERENCES BETWEEN PROTOCOL AND REVIEW	131
INDEX TERMS	131

[Diagnostic Test Accuracy Review]

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection

Jacqueline Dinnes^{1,2}, Jonathan J Deeks^{1,2}, Ada Adriano¹, Sarah Berhane², Clare Davenport^{1,2}, Sabine Dittrich³, Devy Emperador³, Yemisi Takwoingi^{1,2}, Jane Cunningham⁴, Sophie Beese¹, Janine Dretzke¹, Lavinia Ferrante di Ruffano¹, Isobel M Harris¹, Malcolm J Price¹, Sian Taylor-Phillips⁵, Lotty Hooft⁶, Mariska MG Leeftang^{7,8}, René Spijker^{6,9}, Ann Van den Bruel¹⁰, Cochrane COVID-19 Diagnostic Test Accuracy Group²

¹Test Evaluation Research Group, Institute of Applied Health Research, University of Birmingham, Birmingham, UK. ²NIHR Birmingham Biomedical Research Centre, University Hospitals Birmingham NHS Foundation Trust and University of Birmingham, Birmingham, UK. ³FIND, Geneva, Switzerland. ⁴Global Malaria Programme, World Health Organization, Geneva, Switzerland. ⁵Division of Health Sciences, Warwick Medical School, University of Warwick, Coventry, UK. ⁶Cochrane Netherlands, Julius Center for Health Sciences and Primary Care, University Medical Center Utrecht, Utrecht University, Utrecht, Netherlands. ⁷Department of Clinical Epidemiology, Biostatistics and Bioinformatics, Amsterdam University Medical Centers, University of Amsterdam, Amsterdam, Netherlands. ⁸Biomarker and Test Evaluation Programme (BiTE), Amsterdam UMC, University of Amsterdam, Amsterdam, Netherlands. ⁹Medical Library, Amsterdam UMC, University of Amsterdam, Amsterdam Public Health, Amsterdam, Netherlands. ¹⁰Department of Public Health and Primary Care, KU Leuven, Leuven, Belgium

Contact address: Jonathan J Deeks, j.deeks@bham.ac.uk.

Editorial group: Cochrane Infectious Diseases Group.

Publication status and date: New, published in Issue 8, 2020.

Citation: Dinnes J, Deeks JJ, Adriano A, Berhane S, Davenport C, Dittrich S, Emperador D, Takwoingi Y, Cunningham J, Beese S, Dretzke J, Ferrante di Ruffano L, Harris IM, Price MJ, Taylor-Phillips S, Hooft L, Leeftang MMG, Spijker R, Van den Bruel A. Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection. *Cochrane Database of Systematic Reviews* 2020, Issue 8. Art. No.: CD013705. DOI: [10.1002/14651858.CD013705](https://doi.org/10.1002/14651858.CD013705).

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration. This is an open access article under the terms of the [Creative Commons Attribution-Non-Commercial Licence](https://creativecommons.org/licenses/by-nc/4.0/), which permits use, distribution and reproduction in any medium, provided the original work is properly cited and is not used for commercial purposes.

ABSTRACT

Background

Severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) and the resulting COVID-19 pandemic present important diagnostic challenges. Several diagnostic strategies are available to identify or rule out current infection, identify people in need of care escalation, or to test for past infection and immune response. Point-of-care antigen and molecular tests to detect current SARS-CoV-2 infection have the potential to allow earlier detection and isolation of confirmed cases compared to laboratory-based diagnostic methods, with the aim of reducing household and community transmission.

Objectives

To assess the diagnostic accuracy of point-of-care antigen and molecular-based tests to determine if a person presenting in the community or in primary or secondary care has current SARS-CoV-2 infection.

Search methods

On 25 May 2020 we undertook electronic searches in the Cochrane COVID-19 Study Register and the COVID-19 Living Evidence Database from the University of Bern, which is updated daily with published articles from PubMed and Embase and with preprints from medRxiv and bioRxiv. In addition, we checked repositories of COVID-19 publications. We did not apply any language restrictions.

Selection criteria

We included studies of people with suspected current SARS-CoV-2 infection, known to have, or not to have SARS-CoV-2 infection, or where tests were used to screen for infection. We included test accuracy studies of any design that evaluated antigen or molecular tests suitable for a point-of-care setting (minimal equipment, sample preparation, and biosafety requirements, with results available within two hours of sample collection). We included all reference standards to define the presence or absence of SARS-CoV-2 (including reverse transcription polymerase chain reaction (RT-PCR) tests and established clinical diagnostic criteria).

Data collection and analysis

Two review authors independently screened studies and resolved any disagreements by discussion with a third review author. One review author independently extracted study characteristics, which were checked by a second review author. Two review authors independently extracted 2x2 contingency table data and assessed risk of bias and applicability of the studies using the QUADAS-2 tool. We present sensitivity and specificity, with 95% confidence intervals (CIs), for each test using paired forest plots. We pooled data using the bivariate hierarchical model separately for antigen and molecular-based tests, with simplifications when few studies were available. We tabulated available data by test manufacturer.

Main results

We included 22 publications reporting on a total of 18 study cohorts with 3198 unique samples, of which 1775 had confirmed SARS-CoV-2 infection. Ten studies took place in North America, two in South America, four in Europe, one in China and one was conducted internationally. We identified data for eight commercial tests (four antigen and four molecular) and one in-house antigen test. Five of the studies included were only available as preprints.

We did not find any studies at low risk of bias for all quality domains and had concerns about applicability of results across all studies. We judged patient selection to be at high risk of bias in 50% of the studies because of deliberate over-sampling of samples with confirmed COVID-19 infection and unclear in seven out of 18 studies because of poor reporting. Sixteen (89%) studies used only a single, negative RT-PCR to confirm the absence of COVID-19 infection, risking missing infection. There was a lack of information on blinding of index test ($n = 11$), and around participant exclusions from analyses ($n = 10$). We did not observe differences in methodological quality between antigen and molecular test evaluations.

Antigen tests

Sensitivity varied considerably across studies (from 0% to 94%): the average sensitivity was 56.2% (95% CI 29.5 to 79.8%) and average specificity was 99.5% (95% CI 98.1% to 99.9%; based on 8 evaluations in 5 studies on 943 samples). Data for individual antigen tests were limited with no more than two studies for any test.

Rapid molecular assays

Sensitivity showed less variation compared to antigen tests (from 68% to 100%), average sensitivity was 95.2% (95% CI 86.7% to 98.3%) and specificity 98.9% (95% CI 97.3% to 99.5%) based on 13 evaluations in 11 studies of on 2255 samples. Predicted values based on a hypothetical cohort of 1000 people with suspected COVID-19 infection (with a prevalence of 10%) result in 105 positive test results including 10 false positives (positive predictive value 90%), and 895 negative results including 5 false negatives (negative predictive value 99%).

Individual tests

We calculated pooled results of individual tests for ID NOW (Abbott Laboratories) (5 evaluations) and Xpert Xpress (Cepheid Inc) (6 evaluations). Summary sensitivity for the Xpert Xpress assay (99.4%, 95% CI 98.0% to 99.8%) was 22.6 (95% CI 18.8 to 26.3) percentage points higher than that of ID NOW (76.8%, 95% CI 72.9% to 80.3%), whilst the specificity of Xpert Xpress (96.8%, 95% CI 90.6% to 99.0%) was marginally lower than ID NOW (99.6%, 95% CI 98.4% to 99.9%; a difference of -2.8% (95% CI -6.4 to 0.8))

Authors' conclusions

This review identifies early-stage evaluations of point-of-care tests for detecting SARS-CoV-2 infection, largely based on remnant laboratory samples. The findings currently have limited applicability, as we are uncertain whether tests will perform in the same way in clinical practice, and according to symptoms of COVID-19, duration of symptoms, or in asymptomatic people. Rapid tests have the potential to be used to inform triage of RT-PCR use, allowing earlier detection of those testing positive, but the evidence currently is not strong enough to determine how useful they are in clinical practice.

Prospective and comparative evaluations of rapid tests for COVID-19 infection in clinically relevant settings are urgently needed. Studies should recruit consecutive series of eligible participants, including both those presenting for testing due to symptoms and asymptomatic people who may have come into contact with confirmed cases. Studies should clearly describe symptomatic status and document time from symptom onset or time since exposure. Point-of-care tests must be conducted on samples according to manufacturer instructions for use and be conducted at the point of care. Any future research study report should conform to the Standards for Reporting of Diagnostic Accuracy (STARD) guideline.

PLAIN LANGUAGE SUMMARY

How accurate are rapid tests, performed during a health-care visit (point-of-care), for diagnosing COVID-19?

Why is this question important?

People with suspected COVID-19 need to know quickly whether they are infected, so that they can self-isolate, receive treatment, and inform close contacts. Currently, COVID-19 infection is confirmed by sending away samples, taken from the nose and throat, for laboratory testing. The laboratory test, called RT-PCR, requires specialist equipment, may require repeat healthcare visits, and typically takes at least 24 hours to produce a result.

Rapid point-of-care tests can provide a result 'while you wait', ideally within two hours of providing a sample. This could help people isolate early and reduce the spread of infection.

What did we want to find out?

We were interested in two types of rapid point-of-care tests, antigen and molecular tests. Antigen tests identify proteins on the virus, often using disposable devices. Molecular tests detect the virus's genetic material, using small portable or table-top devices. Both test the same nose or throat samples as RT-PCR tests.

We wanted to know whether rapid point-of-care antigen and molecular tests are accurate enough to replace RT-PCR for diagnosing infection, or to select people for further testing if they have a negative result.

What did we do?

We looked for studies that measured the accuracy of rapid point-of-care tests compared with RT-PCR tests to detect current COVID-19 infection. Studies could assess any rapid antigen or molecular point-of-care test, compared with a reference standard test. The reference standard is the best available method for diagnosing the infection; we considered RT-PCR test results and clinically defined COVID-19 as reference tests. People could be tested in hospital or the community. Studies could test people with or without symptoms.

Tests had to use minimal equipment, be performed safely without risking infection from the sample, and have results available within two hours of the sample being collected. Tests could be used in small laboratories or wherever the patient is (in primary care, urgent care facilities, or in hospital).

How did studies assess diagnostic test accuracy?

Studies tested participants with the rapid point-of-care tests. Participants were classified as known to have – and not to have – COVID-19, by RT-PCR in all studies. Studies then identified false positive and false negative errors in the point-of-care test results, compared to RT-PCR. False positive tests incorrectly identified COVID-19 when it was not present, potentially leading to unnecessary self-isolation and further testing. False negatives missed COVID-19 when it was present, risking delayed self-isolation and treatment, and spread of infection.

What we found

We found 18 relevant studies. Ten studies took place in North America, four in Europe, two in South America, one in China and one in multiple countries.

Nine studies deliberately included a high percentage of people with confirmed COVID-19 or included only people with COVID-19. Fourteen studies did not provide any information about the people providing the samples for testing and 12 did not provide any information about where people were tested.

None of the studies reported included samples from people without symptoms.

Main results

Five studies reported eight evaluations of five different antigen tests. Overall, there was considerable variation between the results of the antigen tests in how well they detected COVID-19 infection. Tests gave false positive results in less than 1% of samples.

Thirteen evaluations of four different molecular tests correctly detected an average of 95% of samples with COVID-19 infection. Around 1% of samples gave false positive results.

If 1000 people had molecular tests, and 100 (10%) of them really had COVID-19:

- 105 people would test positive for COVID-19. Of these, 10 people (10%) would not have COVID-19 (false positive result).
- 895 people would test negative for COVID-19. Of these, 5 people (1%) would actually have COVID-19 (false negative result).

We noted a large difference in COVID-19 detection between the two most commonly evaluated molecular tests.

How reliable were the results of the studies?

Our confidence in the evidence is limited.

- Three-quarters of studies did not follow the test manufacturers' instructions, so may have found different results if they had.
- Often, studies did not use the most reliable methods or did not report enough information for us to judge their methods. This may have affected estimates of test accuracy, but it is impossible to identify by how much.
- A quarter of studies were published early online as 'preprints' and are included in the review. Preprints do not undergo the normal rigorous checks of published studies, so we are uncertain how reliable they are.

What are the implications of this review?

Studies provided little information about their participants, so it is not possible to tell if the results can be applied to people with no symptoms, mild symptoms, or who were hospitalised with COVID-19. Accurate rapid tests would have the potential to select people for RT-PCR testing or to be used where RT-PCR is not available. However, the evidence currently is not strong enough and more studies are urgently needed to be able to say if these tests are good enough to be used in practice.

How up-to-date is this review?

This review includes evidence published up to 25 May 2020. Because new research is being published in this field, we will update this review soon.

SUMMARY OF FINDINGS

Summary of findings 1. Diagnostic accuracy of point-of-care antigen and molecular-based tests for the diagnosis of SARS-CoV-2 infection

Question	What is the diagnostic accuracy of rapid point-of-care antigen and molecular-based tests for the diagnosis of SARS-CoV-2 infection?		
Population	<p>Adults or children suspected of:</p> <ul style="list-style-type: none"> current SARS-CoV-2 infection <p>or populations undergoing screening for SARS-CoV-2 infection, including</p> <ul style="list-style-type: none"> asymptomatic contacts of confirmed COVID-19 cases community screening 		
Index test	<p>Any rapid antigen or molecular-based test for diagnosis of SARS-CoV-2 meeting the following criteria:</p> <ul style="list-style-type: none"> portable or mains-powered device minimal sample preparation requirements minimal biosafety requirements no requirement for a temperature-controlled environment test results available within 2 hours of sample collection 		
Target condition	Detection of current SARS-CoV-2 infection		
Reference standard	<p>For COVID-19 cases: positive RT-PCR alone or clinical diagnosis of COVID-19 based on established guidelines or combinations of clinical features</p> <p>For non-COVID-19 cases: repeated negative RT-PCR or pre-pandemic sources of samples</p>		
Action	<p>False negative results mean missed cases of COVID-19 infection, with either delayed or no confirmed diagnosis and increased risk of community transmission due to false sense of security</p> <p>False positive results lead to unnecessary self-isolation or quarantine, with the potential for new infection to be acquired</p>		
Quantity of evidence	Number of studies	Total samples	Total samples with confirmed SARS-CoV-2
	18	3198	1775
Limitations in the evidence			
Risk of bias	<p>Participants: high or unclear risk in 16 studies (89%)</p> <p>Index test: high or unclear risk in 14 studies (78%)</p>		

Reference standard: unclear risk in 10 studies (56%)

Flow and timing: high or unclear risk in 15 studies (83%)

Concerns about applicability

Participants: high concerns in 13 studies (72%)

Index test: high concerns in 13 studies (72%)

Reference standard: high concerns in 17 studies (94%)

Findings

Antigen tests

Evaluations (studies)	Samples	Confirmed SARS-CoV-2 samples	Average sensitivity (95% CI) [Range]	Average specificity (95% CI) [Range]
8 (5)	943	596	56.2 (29.5 to 79.8) [0% to 94%] ^a	99.5 (98.1 to 99.9) [90% to 100%]

Average sensitivity and specificity applied to a hypothetical cohort of 1000 patients ^a

Prevalence of COVID-19	TP	FP	FN	TN	PPV ^b	NPV ^c
5%	28 ^a	5	22 ^a	945	85% (68% to 95%) ^a	98% (97% to 99%)
10%	56 ^a	5	44 ^a	896	92% (82% to 97%) ^a	95% (94% to 97%) ^a
20%	112 ^a	4	88 ^a	796	97% (91% to 99%) ^a	90% (88% to 92%) ^a

Rapid molecular tests

Evaluations (studies)	Samples	Confirmed SARS-CoV-2 samples	Average sensitivity (95% CI) [Range]	Average specificity (95% CI) [Range]
13 (11)	2255	1179	95.2 (86.7 to 98.3) [68% to 100%]	98.9 (97.3 to 99.5) [92% to 100%]

Average sensitivity and specificity applied to a hypothetical cohort of 1000 patients

Prevalence of COVID-19	TP	FP	FN	TN	PPV ^b (95% CI)	NPV ^c (95% CI)
5%	48	10	2	940	83% (71% to 91%)	100% (99% to 100%)
10%	95	10	5	890	90% (83% to 95%)	99% (99% to 100%)
20%	190	9	10	791	95% (92% to 98%)	99% (98% to 99%)
Pooled results for individual tests						
Tests	Evaluations		Samples	SARS-CoV-2 cases	Sensitivity (95% CI)	Specificity (95% CI)
Shenzhen Bioeasy Ag assay	2		238	162	89.5 (83.7 to 93.8)	100 (95.3 to 100)
ID NOW	5		1003	496	76.8 (72.9 to 80.3)	99.6 (98.4 to 99.9)
Xpert Xpress	6		919	479	99.4 (98.0 to 99.8)	96.8 (90.6 to 99.0)
Average sensitivity and specificity applied to a hypothetical cohort of 1000 patients where 100 have COVID-19 infection (10% prevalence)						
Tests	TP	FP	FN	TN	PPV ^b (95% CI)	NPV ^c (95% CI)
Shenzhen Bioeasy Ag assay	90	0	11	900	100% (96% to 100%)	99% (98% to 99%)
ID NOW	77	4	23	896	96% (89% to 99%)	97% (96% to 98%)
Xpert Xpress	99	29	1	871	77% (69% to 84%)	100% (99% to 100%)
Ag: antigen;CI: confidence interval; FN: false negative; FP: false positive;NPV: negative predictive value; PPV: positive predictive value; RT-PCR: reverse transcription polymerase chain reaction; TN: true negative; TP: true positive						

^aAs there is high heterogeneity in the estimates of sensitivity, the values observed in practice could vary considerably from these figures.

^bPPV (positive predictive value) defined as the percentage of positive rapid test results that are truly positive according to the reference standard diagnosis.

^cNPV (negative predictive value) defined as the percentage of negative rapid test results that are truly negative according to the reference standard diagnosis.

BACKGROUND

Severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) and the resulting COVID-19 pandemic present important diagnostic evaluation challenges. These range from: understanding the value of signs and symptoms in predicting possible infection; assessing whether existing biochemical and imaging tests can identify infection or people needing critical care; and evaluating whether new biomarker tests can accurately identify current infection, rule out infection, identify people in need of care escalation, or test for past infection and immunity.

We are creating and maintaining a suite of living systematic reviews to cover the roles of tests and patient characteristics in the diagnosis of COVID-19. This review summarises evidence for the accuracy of rapid antigen and molecular tests, suitable for use at the point of care, as alternatives to standard laboratory-based reverse transcription polymerase chain reaction (RT-PCR), that are relied on for identifying current infection. If sufficiently accurate, point-of-care tests may have a greater impact on public health than RT-PCR as they do not require the same technical expertise and laboratory capacity. These tests can be undertaken locally, avoiding the need for centralised testing facilities that rarely meet the needs of patients, caregivers, health workers and society as a whole, especially in low- and middle-income countries. As these are rapid tests, their results can be returned within the same clinical encounter, facilitating timely decisions concerning the need for isolation.

Target condition being diagnosed

COVID-19 is the disease caused by infection with the SARS-CoV-2 virus. The key target conditions for this suite of reviews are current SARS-CoV-2 infection, current COVID-19 disease, and past SARS-CoV-2 infection. The tests included in this review concern the identification of current infection.

For current infection, the severity of the disease is of importance. SARS-CoV-2 infection can be asymptomatic (no symptoms); mild or moderate (symptoms such as fever, cough, aches, lethargy but without difficulty breathing at rest); severe (symptoms with breathlessness and increased respiratory rate indicative of pneumonia); or critical (requiring respiratory support due to severe acute respiratory syndrome (SARS) or acute respiratory distress syndrome (ARDS). People with COVID-19 pneumonia (severe or critical disease) require different patient management, and it is important to be able to identify them. Viral load may also be an indicator of disease severity (Zheng 2020), and whilst the accuracy of antigen and molecular tests have the potential to be affected by participant viral load, the main aim of rapid testing is not to establish viral load. In this review, we therefore consider the role of point-of-care tests for detecting SARS-CoV-2 infection of any severity.

Index test(s)

The primary consideration for the eligibility of tests for inclusion in this review is that they should detect current infection and should have the capacity to be performed at the 'point of care' or in a 'near-patient' testing role. There is an ongoing debate around the specific use and definitions of these terms, therefore for the purposes of this review, we consider 'point-of-care' and 'near patient' to be

synonymous, but for consistency and avoidance of confusion, we use the term 'point-of-care' throughout.

We have adapted a definition of point-of-care testing, namely that it "refers to decentralized testing that is performed by a minimally trained healthcare professional near a patient and outside of central laboratory testing" (WHO 2018), with the additional caveat that test results must be available within a single clinical encounter (Pai 2012). The key criteria for test inclusion are therefore:

- the equipment for running and or reading the assay must be portable or easily transported, although mains power may be required;
- minimal sample preparation requirements, for example, single-step mixing, with no requirement for additional equipment or precise sample volume transfer unless a disposable automatic fill or graduated transfer device is used;
- minimal biosafety requirements, for example, personal protective equipment (PPE) for sample collector and test operator, good ventilation and a biohazard bag for waste disposal;
- no requirement for a temperature-controlled environment; and
- test results available within two hours of sample collection.

Tests for detection of current infection that are currently suitable for use at the point of care include antigen tests and molecular-based tests. Both types of test use the same respiratory-tract samples acquired by swabbing, washing or aspiration as for laboratory-based RT-PCR. Rapid antigen tests use lateral flow immunoassays, which are disposable devices, usually in the form of plastic cassettes akin to a pregnancy test. Viral antigen is captured by dedicated antibodies that are either colloidal gold- or fluorescent-labelled. Antigen detection is indicated by visible lines appearing on the test strip (colloidal gold-based immunoassays, or CGIA), or through fluorescence, which can be detected using an immunofluorescence analyser (fluorescence immunoassays or FIA). Molecular-based tests to detect viral ribonucleic acid (RNA) have historically been laboratory-based assays using RT-PCR technology (see Alternative test(s)). In recent years, automated, single-step RT-PCR methods have been developed, as well as other nucleic acid amplification methods, such as isothermal amplification, that do not require the sophisticated thermo cycling involved in RT-PCR (Carter 2020). These technological advances have allowed molecular technologies to be developed that are suitable for use in a point-of-care context (Kozel 2017).

Following the emergence of COVID-19 there has been prolific industry activity to develop accurate tests. The Foundation for Innovative Diagnostics (FIND) and Johns Hopkins Centre for Health Security have maintained online lists of these and other molecular-based tests for SARS-CoV-2 (FIND 2020). At the time of writing (19 July 2020), FIND listed 48 rapid antigen tests, 32 of which are described as "commercialized" and 21 have been identified as having regulatory approval. A total of 113 molecular tests were described as automated, including both laboratory-based assays and assays suitable for use outside of a laboratory setting (i.e. near or at the point of care). Further information from FIND indicates that 47 of the 113 assays were categorised as point-of-care or near point-of-care tests, including 26 with regulatory approval. This classification was based on the information provided to FIND by the test manufacturers and does not necessarily mean that these tests meet the criteria for point-of-care tests that we have specified for

this review. The numbers of tests of these types will increase over time.

Clinical pathway

Patients may be tested for infection when they present with symptoms, or have had known exposure to COVID-19, or during screening for COVID-19. The standard approach to diagnosis of COVID-19 infection is through laboratory-based testing of swab samples taken from the upper respiratory (e.g. nasopharynx, oropharynx) or lower respiratory tract (e.g. bronchoalveolar lavage or sputum) with RT-PCR. RT-PCR is the primary method for detecting infection during the acute phase of the illness while the virus is still present (whether people are symptomatic or asymptomatic), but can give false negative results ([Arevalo-Rodriguez 2020](#)). Both the World Health Organisation (WHO) and the China CDC (National Health Commission of the People's Republic of China), have produced case definitions for COVID-19 that include the presence of convincing clinical evidence when RT-PCR is negative ([Appendix 1](#)). The most recent case definition from the China CDC also includes positive serology tests.

Prior test(s)

Signs and symptoms are used in the initial diagnosis of suspected COVID-19 infection and to help identify those who require a test for RT-PCR. A number of key symptoms have been associated with mild to moderate COVID-19, including: troublesome dry cough (for example, coughing more than usual over a one-hour period, or three or more coughing episodes in 24 hours), fever greater than 37.8 °C, diarrhoea, headache, breathlessness on light exertion, muscle pain, fatigue, and loss of sense of smell and taste. However, the recently published review of signs and symptoms found good evidence for the accuracy for these symptoms alone or in combination to be lacking ([Struyf 2020](#)).

Where people are asymptomatic but are being tested on the basis of epidemiological risk factors, such as exposure to someone with confirmed SARS-CoV-2, no prior tests will have been conducted.

Role of index test(s)

For most settings in which testing for acute SARS-CoV-2 infection takes place, results of laboratory-based RT-PCR tests are unlikely to be available within a single clinical encounter. Point-of-care tests potentially have a role either as a replacement for RT-PCR (if sufficiently accurate), or as a means of triaging and rapid management (quarantine or treatment, or both), with confirmatory RT-PCR testing for negative results. Obtaining quick results within a healthcare visit will allow more appropriate decisions about isolation and healthcare interventions. If accurate, tests may also be considered for screening at-risk populations, for example in airport settings or in local outbreaks.

Alternative test(s)

This review is one of seven planned reviews that cover the range of tests and characteristics being considered in the management of COVID-19 ([Deeks 2020](#); [McInnes 2020](#)). Full details of the alternative tests and evidence of their accuracy will be summarised in these reviews. Tests that might be considered as alternatives to point-of-care tests are considered here.

Laboratory-based molecular tests

RT-PCR tests for SARS-CoV-2 identify viral ribonucleic acid (RNA). Reagents for RT-PCR were rapidly produced once the viral RNA sequence was published ([Corman 2020](#)). Testing is undertaken in central laboratories and can be very labour-intensive, with several points along the path of performing a single test where errors may occur, although some automation of parts of the process is possible. The amplification process requires thermal cycling equipment to allow multiple temperature changes within a cycle, with cycles repeated up to 40 times until viral DNA is detected ([Carter 2020](#)). Although the amplification process for RT-PCR can be completed in a relatively short timeframe, the stages of extraction, sample processing and data management (including reporting) mean that test results are typically only available in 24 to 48 hours. Where testing is undertaken in a centralised laboratory, transport times increase this further. The time to result for fully automated RT-PCR assays is shorter than for manual RT-PCR, however most assays still require sample preparation steps that make them unsuitable for use at the point of care. Other nucleic acid amplification methods, including loop-mediated isothermal amplification (LAMP), or CRISPR-based nucleic acid detection methods, that allow amplification at a constant temperature are also being developed ([Carter 2020](#)). These methods have the potential to reduce the time to produce test results after extraction and sample processing to minutes, but the time for the whole process may still be significant. Laboratory-based molecular tests are most often applied to upper and lower respiratory samples although they are also being used on faecal and urine samples.

Antibody tests

Serology tests to measure antibodies to SARS-CoV-2 have been evaluated in people with active infection and in convalescent cases ([Deeks 2020a](#)). Antibodies are formed by the body's immune system in response to infections, and can be detected in whole blood, plasma or serum. Antibody tests are available for laboratory use including enzyme-linked immunosorbent assay (ELISA) methods, or more advanced chemiluminescence immunoassays (CLIA). There are also rapid lateral flow assays (LFA)s for antibody testing that use a minimal amount of whole blood, plasma or serum on a testing strip as opposed to the respiratory specimens that are used for rapid antigen tests; all assays for antibody detection are considered in [Deeks 2020a](#).

Rationale

It is essential to understand the clinical accuracy of tests and diagnostic features to identify the best way they can be used in different settings to develop effective diagnostic and management pathways. The suite of Cochrane 'living systematic reviews' summarises evidence on the clinical accuracy of different tests and diagnostic features, grouped according to the research questions and settings that we are aware of. Estimates of accuracy from these reviews will help inform diagnosis, screening, isolation, and patient-management decisions.

As the COVID-19 pandemic progresses, earlier, fast and reliable detection of active SARS-CoV-2 infection is key to reducing community transmission. New biomarker tests are being developed and evidence is accumulating at an unprecedented rate. Point-of-care testing provides a potentially attractive route to increasing testing rates; however their potential to have an impact on patient care and help reduce transmission depends not only on

the time it takes to report the test result, but on test performance and frequency of testing. We are aware of two other reviews on this topic (Green 2020; Subsoontorn 2020). One rapid review of point-of-care tests relied on performance data from manufacturers' instructions for use documents (Green 2020). A systematic review of nucleic acid amplification 'point-of-care tests' selected studies for inclusion based on the use of isothermal techniques (i.e. not requiring thermal cycling), with apparently no consideration for the feasibility of deploying the tests in a point-of-care environment (Subsoontorn 2020). A comprehensive systematic review of the clinical performance of tests suitable for use at the point of care is therefore urgently needed. We will update this review as often as is feasible to ensure that it provides current evidence about the accuracy of point-of-care tests.

Please note, this review follows a generic protocol that covers six of the seven Cochrane COVID-19 DTA reviews (Deeks 2020). The Background and Methods sections of this review therefore use some text that was originally published in the protocol (Deeks 2020), and text that overlaps some of our other reviews (Deeks 2020a; Struyf 2020).

OBJECTIVES

To assess the diagnostic accuracy of rapid point-of-care antigen and molecular-based tests to determine if a person presenting in the community or in primary or secondary care has current SARS-CoV-2 infection.

Secondary objectives

Where data are available, we will investigate potential sources of heterogeneity that may influence diagnostic accuracy (either by stratified analysis or meta-regression) according to index test, participant characteristics (length and severity of symptoms, and viral load), study setting, study design and reference standard used.

METHODS

Criteria for considering studies for this review

Types of studies

We applied broad eligibility criteria in order to include all patient groups (that is, if patient population was unclear, we included the study) and all variations of a test.

We included studies of all designs that produce estimates of test accuracy or provide data from which we can compute estimates, including the following.

- Studies restricted to participants confirmed to either have (or to have had) the target condition (to estimate sensitivity) or confirmed not to have (or have had) the target condition (to estimate specificity). These types of studies may be excluded in later review updates.
- Single-group studies, which recruit participants before disease status has been ascertained.
- Multi-group studies, where people with and without the target condition are recruited separately (often referred to as two-gate or diagnostic case-control studies).
- Studies based on either patients or samples.

We excluded studies from which we could not extract data to compute either sensitivity or specificity.

We carefully considered the limitations of different study designs in the quality assessment and analyses.

We included studies reported in published articles and as preprints.

Participants

We included studies recruiting people presenting with suspicion of current SARS-CoV-2 infection or those recruiting populations where tests were used to screen for disease (for example, contact tracing or community screening).

We also included studies that recruited people known to have SARS-CoV-2 infection and known not to have SARS-CoV-2 infection (i.e. cases only or multi-group studies).

We excluded small studies with fewer than 10 samples or participants. Although the size threshold of 10 is arbitrary, such small studies are likely to give unreliable estimates of sensitivity or specificity and may be biased.

Index tests

We included studies evaluating any rapid antigen or molecular-based test for diagnosis of SARS-CoV-2, if it met the criteria outlined in the Background, that is, requiring minimal equipment, sample preparation, and biosafety considerations, with results available within two hours of sample collection.

Target conditions

The target condition was current SARS-CoV-2 infection (either symptomatic or asymptomatic). We also refer to SARS-CoV-2 infection as 'COVID-19 infection'.

Reference standards

We anticipated that studies would use a range of reference standards to define both the presence and absence of SARS-CoV-2 infection but were unclear at the start of the review exactly what methods we would encounter. For the QUADAS-2 (Quality Assessment tool for Diagnostic Accuracy Studies; Whiting 2011), assessment we categorised each method of defining the presence of SARS-CoV-2 according to the risk of bias (the chances that it would misclassify the presence or absence of infection) and whether it defined COVID-19 in an appropriate way that reflected cases encountered in practice. Likewise, we considered the risk of bias in definitions of the absence of SARS-CoV-2, and whether the definition included all those who would be tested in practice.

Evaluations of molecular tests generally consider agreement between molecular assays, for example, agreement of a new rapid test against a more standard RT-PCR test. For the purposes of this review, we considered RT-PCR to be the 'reference standard' against which the rapid tests were compared, and present results as 'sensitivity' and 'specificity' as opposed to percentage agreement. The result of further RT-PCR analysis of discrepant cells (samples with results disagreeing on the rapid test and the RT-PCR) were also considered in sensitivity analyses. As discrepant analysis involves retesting only a subsample of patients selected according to index and reference standard results, it can introduce bias (Hadgu 1999). Retesting of all samples with a second test in a composite reference

standard would be preferable when there are concerns over the accuracy of the first reference test.

Search methods for identification of studies

Electronic searches

We conducted a single literature search to cover our suite of Cochrane COVID-19 diagnostic test accuracy (DTA) reviews (Deeks 2020; McInnes 2020).

We conducted electronic searches using two primary sources. Both of these searches aimed to identify all published articles and preprints related to COVID-19, and were not restricted to those evaluating biomarkers or tests. Thus, there are no test terms, diagnosis terms, or methodological terms in the searches. Searches were limited to 2019 and 2020, and for this version of the review have been conducted to 25 May 2020.

Cochrane COVID-19 Study Register searches

We used the Cochrane COVID-19 Study Register (covid-19.cochrane.org/), for searches conducted from inception of the Register to 28 March 2020. At that time, the register was populated by searches of PubMed, as well as trials registers at ClinicalTrials.gov and the WHO International Clinical Trials Registry Platform (ICTRP).

Search strategies were designed for maximum sensitivity, to retrieve all human studies on COVID-19 and with no language limits. See [Appendix 2](#).

COVID-19 Living Evidence Database from the University of Bern

From 28 March 2020, we used the COVID-19 Living Evidence database from the Institute of Social and Preventive Medicine (ISPM) at the University of Bern (www.ispm.unibe.ch), as the primary source of records for the Cochrane COVID-19 DTA reviews. This search includes PubMed, Embase, and preprints indexed in bioRxiv and medRxiv databases. The strategies as described on the ISPM website are described here (ispmbern.github.io/covid-19/). See [Appendix 3](#). To ensure comprehensive coverage we also downloaded records from the 'Bern feed' from 1 January to 28 March 2020 and de-duplicated them against those obtained via the Cochrane COVID-19 Study Register.

The decision to focus primarily on the Bern feed was because of the exceptionally large numbers of COVID-19 studies available only as preprints. The Cochrane COVID-19 Study Register has undergone a number of iterations since the end of March and we anticipate moving back to the Register as the primary source of records for subsequent review updates.

Searching other resources

We identified Embase records through the Centers for Disease Control and Prevention (CDC), Stephen B Thacker CDC Library, COVID-19 Research Articles Downloadable Database (www.cdc.gov/library/researchguides/2019novelcoronavirus/researcharticles.html), and de-duplicated them against the Cochrane COVID-19 Study Register up to 28 March 2020. See [Appendix 4](#).

We also checked our search results against two additional repositories of COVID-19 publications including:

- the Evidence for Policy and Practice Information and Coordinating Centre (EPPI-Centre) 'COVID-19: Living map of the evidence' (eppi.ioe.ac.uk/COVID19_MAP/covid_map_v4.html);
- the Norwegian Institute of Public Health 'NIPH systematic and living map on COVID-19 evidence' (www.norgesk.no/forskningskart/NIPH_diagnosisMap.html)

Both of these repositories allow their contents to be filtered according to studies potentially relating to diagnosis, and both have agreed to provide us with updates of new diagnosis studies added. For this iteration of the review, we examined all diagnosis studies from either source up to 25 May 2020.

We appeal to researchers to supply details of additional published or unpublished studies at the following email address, which we will consider for inclusion in future updates (covidtda@contacts.bham.ac.uk).

Data collection and analysis

Selection of studies

A team of experienced systematic review authors from the University of Birmingham screened the titles and abstracts of all records retrieved from the literature searches. Two review authors independently screened studies in [Covidence](#). A third, senior review author resolved any disagreements. We tagged all records selected as potentially eligible according to the Cochrane COVID-19 DTA review(s) that they might be eligible for and we then exported them to separate [Covidence](#) reviews for each review title.

We obtained the full texts for all studies flagged as potentially eligible. Two review authors independently screened the full texts for one of the COVID-19 biomarker reviews (molecular, antigen or antibody tests). We resolved any disagreements on study inclusion through discussion with a third review author.

Data extraction and management

One review author extracted the characteristics of each study, which a second review author checked. Items that we extracted are listed in [Appendix 5](#). In addition, we coded tests according to complexity, regardless of the nature of the test (antigen or molecular test), as follows:

- low: one sample preparation step and up to two test steps;
- moderate: two sample preparation steps and up to three test steps;
- high: more than two sample preparation steps and more than three test steps.

Two review authors independently carried out this classification, with referral to a third review author if necessary.

Both review authors independently performed data extraction of 2x2 contingency tables of the number of true positives, false positives, false negatives and true negatives. They resolved disagreements by discussion. Where possible, we separately extracted data according to viral load, and for molecular assays, before and after re-analysis of samples in discrepant cells.

We encourage study authors to contact us regarding missing details on the included studies (covidtda@contacts.bham.ac.uk).

Assessment of methodological quality

Two review authors independently assessed risk of bias and applicability concerns using the QUADAS-2 checklist tailored to this review ([Appendix 6](#); [Whiting 2011](#)). The two review authors resolved any disagreements by discussion.

Ideally, studies should prospectively recruit a representative sample of participants presenting with signs and symptoms of COVID-19, either in community or primary care settings or to a hospital setting, and they should clearly record the time of testing after the onset of symptoms. Studies in asymptomatic people at risk of infection should document time from exposure. Studies should perform tests in their intended use setting, using appropriate samples with or without viral transport medium and within the time period following specimen collection as indicated in the 'instructions for use' document. Tests should be performed by relevant personnel (e.g. healthcare workers), and should be interpreted blinded to the final diagnosis (presence or absence of SARS-CoV-2). The reference standard diagnosis should be blinded to the result of the rapid test, and should not incorporate the result of the index test. We did not consider a comparison of a rapid molecular-based test against an RT-PCR assay to be at risk of incorporation bias. If the reference standard includes clinical diagnosis of COVID-19 for RT-PCR-negative patients, then established criteria should be used. Studies including samples from participants known not to have COVID-19 should use pre-pandemic sources or contemporaneous samples with at least one RT-PCR-negative test result. Data should be reported for all study participants, including those where the result of the rapid test was inconclusive, or participants in whom the final diagnosis of COVID-19 was uncertain. Studies should report whether results relate to participants (one sample per participant), or samples (multiple samples per participant).

Statistical analysis and data synthesis

We analysed rapid antigen and molecular tests separately. If studies evaluated multiple tests in the same samples, we included them multiple times. We present estimates of sensitivity and specificity for each test brand using paired forest plots, and summarise results using average sensitivity and specificity in tables as appropriate. There were only sufficient studies to make formal comparisons (based on between-study comparisons) for studies using two brands of molecular tests (ID NOW (Abbott Laboratories) and Xpert Xpress (Cepheid Inc)).

We estimated summary sensitivities and specificities with 95% confidence intervals (CI) using the bivariate model ([Reitsma 2005](#)), via the `meqrlogit` command of [Stata/SE 16.0](#). When few studies were available, we simplified models by first assuming no correlation between sensitivity and specificity estimates and secondly by setting near-zero variance estimates of the random effects to zero ([Takwoingi 2017](#)). In cases where there was only one study per test, we reported individual sensitivities and specificities with 95% CI constructed using the binomial exact method.

Where studies presented only estimates of sensitivity, we fitted univariate random effects logistic regression models. In a small number of instances where a model failed to converge (usually when there were very small numbers of studies or the sensitivity/specificity estimates were all very high), we computed estimates

and CI by summing the counts of TP, FP, FN and TN across 2x2 tables. These analyses are clearly marked in the tables. We present all estimates with 95% confidence intervals.

Investigations of heterogeneity

We examined heterogeneity between studies by visually inspecting the forest plots of sensitivity and specificity. Where adequate data were available, we investigated heterogeneity related to viral load, test brand, and sample type by including indicator variables in the random-effects logistic regression models. Absolute differences between the sensitivity or specificity and the P values were reported from the model. In instances where only one study was available per test or when tests were being directly compared following summing of counts of the 2x2 tables, we performed test comparison using the two-sample test of proportions.

Sensitivity analyses

We performed three sensitivity analyses. First, estimation of sensitivity for molecular tests was made with and without studies that only evaluated samples with RT-PCR-confirmed SARS-CoV-2 (and thus did not estimate specificity). Secondly, comparisons were made between analyses using the primary reference standard and analyses using results adjusted after sample retesting with a second RT-PCR test, either for discrepant cells (discrepant analysis) or for all samples. Thirdly, we restricted our analysis comparing ID NOW (Abbott Laboratories) and Xpert Xpress (Cepheid Inc) to studies that compared the tests in the same samples.

Assessment of reporting bias

We made no formal assessment of reporting bias.

Summary of findings

We summarised key findings in a 'Summary of findings' table indicating the strength of evidence for each test and findings, and highlighted important gaps in the evidence.

Updating


We are aware of additional studies published since the search date of 25 May 2020 and plan to update this review imminently. We have already completed searches for the update up until 22 June 2020, and screening of those is ongoing.

RESULTS

Results of the search

We screened 19,092 unique records (published or preprints) for inclusion in the complete suite of reviews to assist in the diagnosis of COVID-19 ([Deeks 2020](#); [McInnes 2020](#)). Of 808 records selected for further assessment for inclusion in any of the four molecular, antigen or antibody test reviews, we assessed 90 full-text reports for inclusion in this review. See [Figure 1](#) for the PRISMA flow diagram of search and eligibility results ([McInnes 2018](#); [Moher 2009](#)). We included 18 studies from 22 reports in this review, and we excluded 68 publications that did not meet our inclusion criteria. Exclusions were mainly because of index tests not meeting our criteria for use at the point of care (n = 36) or ineligible study designs (n = 21). The reasons for exclusion of all 68 publications are provided in [Characteristics of excluded studies](#).

Figure 1. Study flow diagram

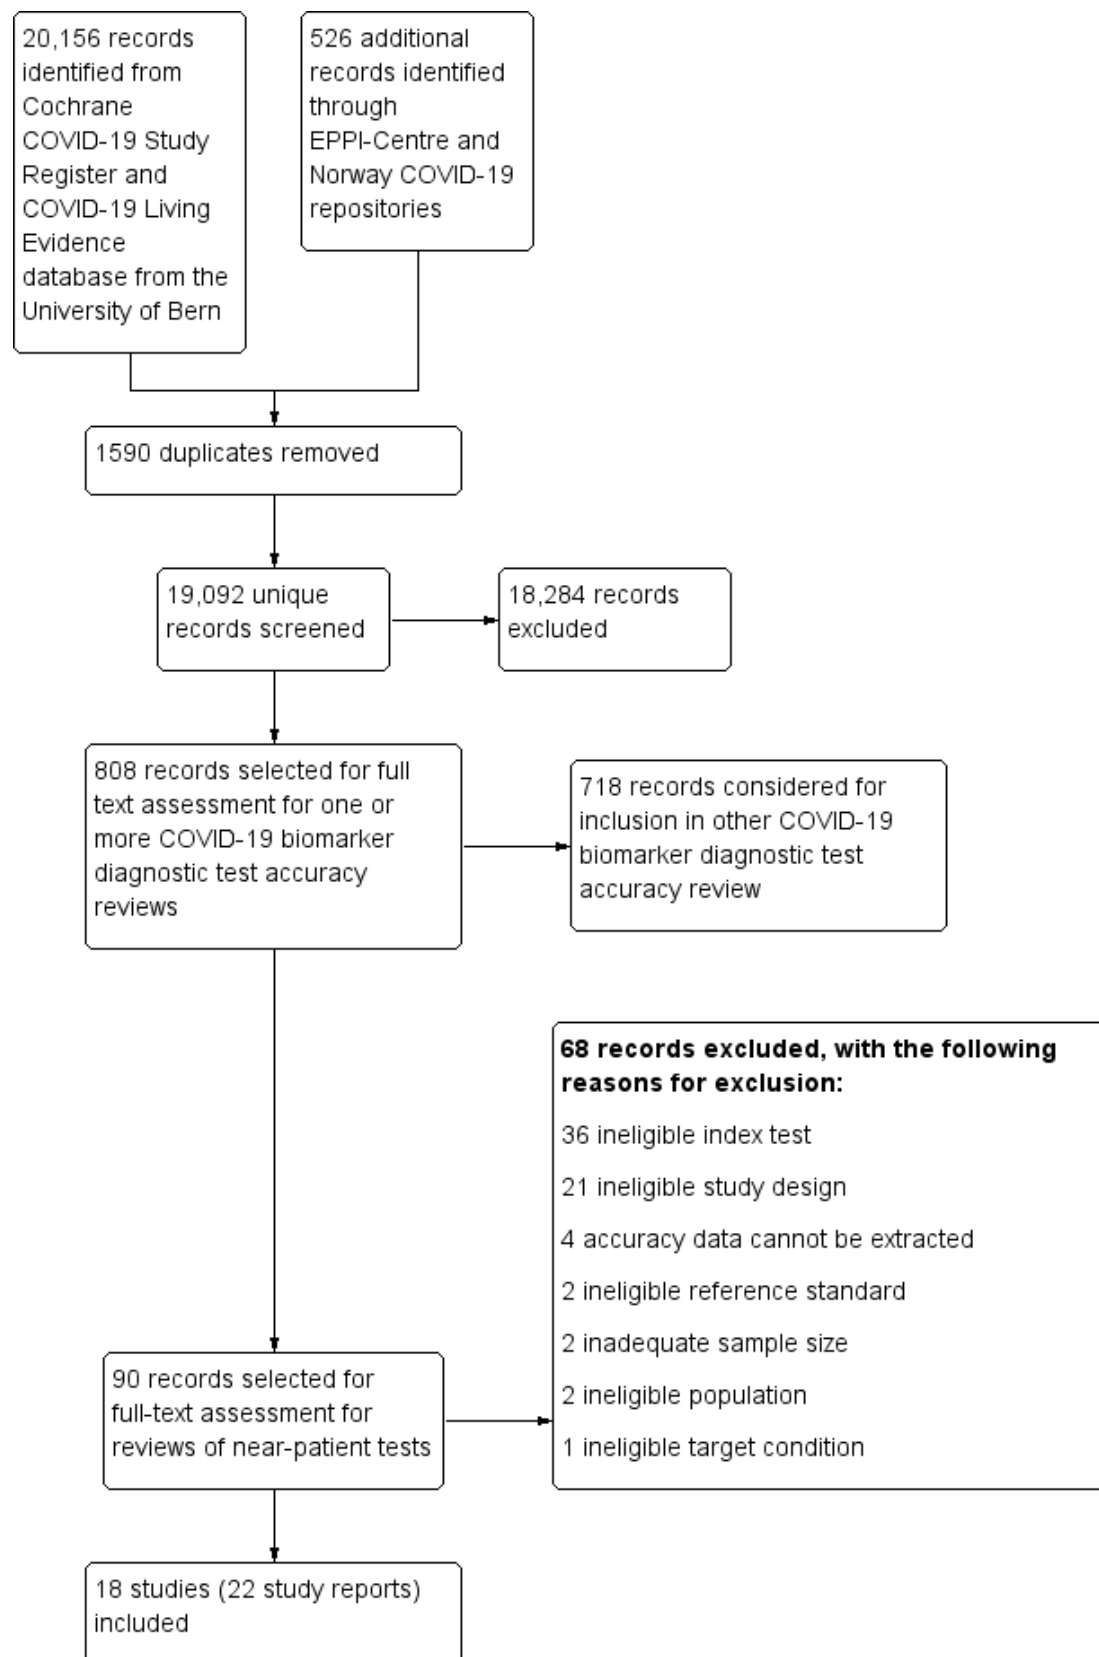

We contacted the authors of three included studies for further information ([Diao 2020](#); [Porte 2020](#); [Weitzel 2020 \[A\]](#)), and received replies and the requested information in regard to all three.

The 22 included study reports relate to 18 separate studies, four studies having both preprints and subsequent journal publications ([Broder 2020](#); [Mertens 2020](#); [Porte 2020](#); [Smithgall 2020 \[A\]](#)). Of the 18 studies, five are available only as preprints. (Please note when naming studies, we use the letters [A], [B], [C] etc. in square brackets to indicate data on different tests evaluated in the same study).

Description of included studies

The 18 studies include a total of 3198 unique samples, with 1775 samples with RT-PCR-confirmed SARS-CoV-2 (some samples were analysed by more than one index test). Five studies evaluated antigen tests ([Diao 2020](#); [Lambert-Niclot 2020](#); [Mertens 2020](#); [Porte 2020](#); [Weitzel 2020 \[A\]](#)) and 13 studies evaluated molecular tests ([Assennato 2020](#); [Broder 2020](#); [Harrington 2020](#); [Hogan 2020](#); [Lieberman 2020](#); [Loeffelholz 2020](#); [Mitchell 2020](#); [Moore 2020](#); [Moran 2020](#); [Rhoads 2020](#); [Smithgall 2020 \[A\]](#); [Wolters 2020](#); [Zhen 2020 \[A\]](#)). Summary study characteristics are presented in [Table 1](#) with further details of study design and index test details in [Appendix 7](#) and [Appendix 8](#). Full details are provided in the [Characteristics of included studies table](#).

The median sample size of the included studies is 112 (interquartile range (IQR) 96 to 198) and median number of SARS-CoV-2 confirmed samples included is 85 (IQR 50 to 119). The majority of studies (10/18) were conducted in the USA, four in Europe, two in South America, one in China and one study included samples from more than one country.

Participant characteristics

Studies predominantly selected samples from those submitted to laboratories for routine RT-PCR testing with limited detail of the participants providing the samples. Three studies included samples from participants in emergency department or urgent care settings, three included samples from participants presenting in mixed settings (inpatient, outpatient or emergency department), and 12 did not report any details of setting in which study participants presented.

Four studies included samples from symptomatic patients, only one of which provided any information on the type of symptoms experienced and time from symptom onset (median 2 days; IQR 1 to 4; range 0 to 12; [Porte 2020](#)). Three additional studies provided basic demographic data such as age or gender, and the remaining 14 provided no information on participant characteristics.

All five studies evaluating antigen tests reported results for SARS-CoV-2-confirmed samples with high and low viral load as defined by the cycle threshold (Ct) value from the reference standard. In one study ([Diao 2020](#)), the proportion with high viral load was 27% (cut-off ≤ 30 Ct), and in the other four (using a cut-off of ≤ 25 Ct) it ranged from 48% to 74% ([Appendix 7](#)). Four studies reporting five molecular assay evaluations, reported proportions with high viral load ranging from 33% ([Mitchell 2020](#)), to 60% ([Smithgall 2020 \[A\]](#)). All four studies defined high viral load as Ct of 30 or less. Ct values were missing for some samples in [Porte 2020](#).

Study designs

We found it difficult to fully ascertain whether samples were included in studies with or without knowledge of whether patients did or did not have COVID-19 infection. All studies defined the presence or absence of COVID-19 infection based on RT-PCR, with a single ($n = 17$) or two ($n = 1$) negative RT-PCR results used to confirm the absence of infection. One study used paired nasopharyngeal swabs for RT-PCR and nasal swabs for the index test ([Harrington 2020](#)); all other studies used the same respiratory sample for the RT-PCR and for the index test.

Nine studies appeared to include series of samples submitted for laboratory testing regardless of the RT-PCR result, but only [Harrington 2020](#) reported including consecutive samples, and only [Mertens 2020](#) randomly selected samples. The number of samples in these single-group studies ranged from 26 to 524 with between 13 and 208 samples with confirmed SARS-CoV-2 (median prevalence 50%; IQR 41% to 68%).

Seven studies described deliberate separate sampling of RT-PCR-positive and RT-PCR-negative samples, for example, to 'enrich' for positive samples, to reach a stated ratio of positive to negative samples, or to represent a range of Ct values on RT-PCR. We designated these studies as two-group studies. Sample sizes of these studies ranged from 88 to 481 with between 57 and 220 samples with confirmed SARS-CoV-2 (median prevalence 60%; IQR 46% to 66%).

Two studies included only samples with confirmed SARS-CoV-2, thus only allowing estimation of sensitivity; 35 samples in [Broder 2020](#), and 96 in [Rhoads 2020](#).

Index tests

Fifteen studies evaluated only one test, three compared two or more tests using the same samples (two with two tests each, and one with four tests). In total the 18 studies reported on a total of 23 test evaluations. [Appendix 9](#) provides details extracted from the manufacturer's instructions for use documents for all included tests.

Antigen tests

Five studies reported eight evaluations of antigen tests (4 CGIA and 4 FIA), seven of which evaluated one of five commercially produced tests (produced by Beijing Savant, Shenzhen Bioeasy, Coris BioConcept, Liming Bio-Products and RapiGEN Inc.) and one classified as using an in-house CGIA method (full identification details for all tests is provided in [Appendix 8](#)). Contact with the study author indicates that this study reports the development of the Shenzhen Bioeasy assay ([Diao 2020](#)), but it is not clear whether the commercially available assay is identical to the one reported in the study or whether it has undergone further refinement. Only two studies provided product codes for the tests evaluated ([Porte 2020](#); [Weitzel 2020 \[A\]](#); [Appendix 8](#)). The Beijing Savant, Coris BioConcept, Shenzhen Bioeasy and in-house assays all target the nucleocapsid protein; this information was not reported for the Liming Bio-Products and RapiGEN Inc. assays ([Appendix 8](#)). We have not been able to identify any information for either the Beijing Savant or Liming Bio-Products assays online.

Two of the five studies used only nasopharyngeal swab samples, two used both nasopharyngeal and oropharyngeal swab samples from all patients ([Porte 2020](#); [Weitzel 2020 \[A\]](#)),

and one study (Mertens 2020), used mixed swab samples including nasopharyngeal swabs, nasopharyngeal aspirate and bronchoalveolar lavage. All studies used samples either in viral transport medium (n = 4) or in saline solution (n = 1; Diao 2020). The Coris BioConcept assay, evaluated in two studies (Lambert-Niclot 2020; Mertens 2020), is the only one to document instructions for use for swabs in viral transport medium (VTM); the use of VTM is not mentioned in the instructions for use documents for any of the other assays (Appendix 9). Samples were tested "soon" after collection in Lambert-Niclot 2020, after a defined period of refrigerated storage in Porte 2020 or frozen storage in Weitzel 2020 [A]; two studies did not report sample storage and timing of testing.

Molecular tests

Thirteen studies reported 15 evaluations of four different commercially available rapid molecular tests: six evaluating ID NOW (Abbott Laboratories), seven evaluating Xpert Xpress (Cepheid Inc), and one evaluation each of Accula (Mesa Biotech Inc.) and SAMBA II (Diagnostics for the Real World). None of the studies reported product codes for the tests evaluated (Appendix 8). One study of Xpert Xpress used the 'research use only' (RUO) version of the test, but reported that the RUO version contains the same reagents as the 'emergency use authorisation' (EUA) version. The RUO test allows the user to view the amplification curves for the RdRp gene as well as for the E-gene and N2 targets whereas the EUA version restricts the amplification curves to E and N2 only. ID NOW and SAMBA-II use isothermal techniques, Xpert Xpress is based on RT-PCR, and Accula is described as a PCR plus LFA.

In the 13 studies, seven used only nasopharyngeal (n = 6) or nasal (n = 1) swab samples, one used both nasopharyngeal and oropharyngeal swab samples from all patients, and the remaining five evaluations used mixed swab samples including nasopharyngeal or nasal swabs (n = 3), nasopharyngeal or oropharyngeal swabs (n = 1), or multiple sample types including

tracheal aspirate (n = 1). One study reported direct swab testing (Harrington 2020), 10 used either swabs in viral transport medium (n = 5), viral transport medium or saline (n = 4), or viral transport medium or gelatin-lactalbumin-yeast (GLY) medium (n = 1), and two did not report whether any transport medium was used. Five of 13 studies reported testing immediately (n = 1), or within 48 (n = 1) or 72 hours (n = 3) of sample collection. Four studies reported testing after a period of frozen storage, and four did not describe sample storage or timing of testing at all. Two of the four manufacturers document instructions for use for samples in transport medium (for the Xpert Xpress and SAMBA II assays) and two explicitly recommend against the use of viral transport medium (ID NOW and Accula), although at the time of the test evaluations, some viral transport media were documented as acceptable for ID NOW. Although immediate sample testing is preferred, all manufacturers document acceptable period of refrigerated storage of between 24 hours (ID NOW) and seven days (Xpert Xpress). See Appendix 9.


Across the 23 test evaluations of antigen or molecular tests, only one reported testing outside of a centralised laboratory setting, where direct swab testing (using ID NOW (Abbott Laboratories)) was carried out by on-site medical personnel or laboratory personnel at local laboratories (Harrington 2020).

Our own assessment of test complexity across test types classified SAMBA II as high complexity (more than two sample preparation steps and more than three test steps), Shenzhen Bioeasy FIA, ID NOW and Accula as moderate complexity and the other antigen tests and Xpert Xpress as low complexity (one sample preparation step and up to two test steps).

Methodological quality of included studies

We report the overall methodological quality assessed using the QUADAS-2 tool for all included studies (n = 18) in Figure 2 (Whiting 2011). See Appendix 10 for a plot of study-level ratings by quality.

Figure 2. Risk of bias and applicability concerns graph: review authors' judgements about each domain presented as percentages across included studies. Numbers in the bars indicate the number of studies

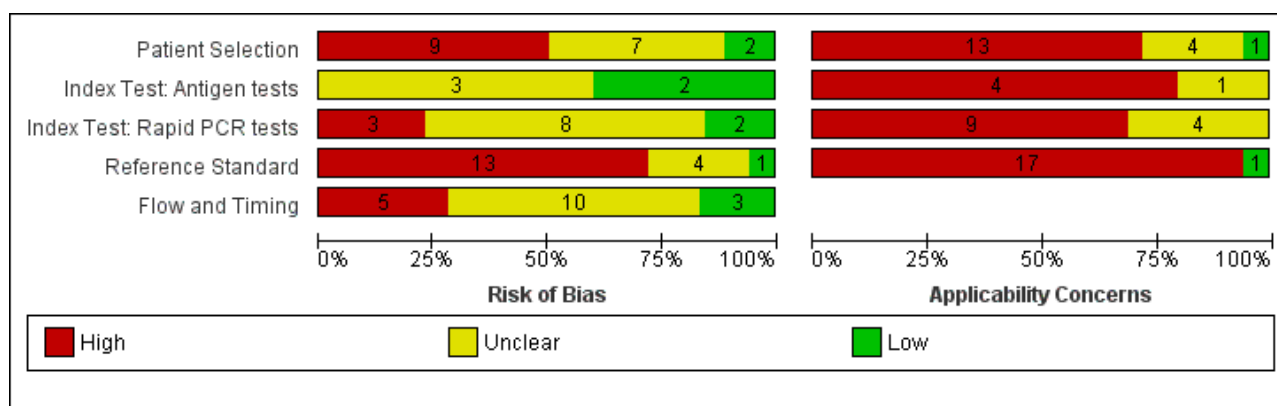

We considered the risk of bias in the individual studies and whether the results were likely to be applicable to standard use of the tests. We did not judge any study at low risk of bias and we had concerns about the applicability of results in all studies. We considered risk of bias to be high in nine (50%) studies because of how they selected samples and in 13 (72%) because they considered that one negative RT-PCR was sufficient to confirm the absence of COVID-19 infection. Lack of details in reporting meant we could not clearly

assess whether there was a risk of bias through performance of the index test in 11 (61%) studies, or from the way in which the study was undertaken and analysed in 10 (56%). We judged that there were high concerns about the applicability of the evidence related to participants in 13 (72%) studies, to the index test in 13 (72%) studies and to the reference standard in 17 (94%) studies. We did not observe differences in methodological quality between antigen and molecular test evaluations. Explanations of how we reached

these judgements are given below and in the [Characteristics of included studies](#) table.

Participant selection

We judged only two studies to be at low risk of bias, and in seven (39%) the risk was unclear because of poor reporting. The remaining 50% (9/18) we judged to be at high risk of bias because of deliberate sampling of participants based on the reference standard result; two of which also only included samples with confirmed COVID-19 infection. We were not able to judge the appropriateness of study exclusions (16/18) or inclusions (11/18) where selection was based on the availability of laboratory samples with no participant eligibility criteria specified. Numbers per group are not mutually exclusive.

We had high concerns about the applicability of the selected participants in 13/18 studies (72%), meaning that the participants who were recruited were unlikely to be similar to those in whom the test would be used in clinical practice. This was largely because of the use of deliberate sampling; and sample inclusion based on the availability of residual and sometimes frozen samples, created unrepresentative participant samples. We judged only one study recruiting participants presenting to urgent care or emergency departments as likely to have selected an appropriate patient group.

Index tests

[Figure 2](#) demonstrates similar patterns in risk of bias and applicability of the index test for studies of both antigen and rapid molecular tests. We observed low risk of bias in four studies that clearly described interpretation of the index test blinded to results of the reference standard, and used prespecified test thresholds. There was high risk of bias in three studies because the manufacturer's prespecified threshold for the Xpert Xpress test (re-testing of samples with presumptive positive results) was not followed. The risk of bias was unclear in 11 studies because we could not judge whether interpretation of the index test was undertaken with knowledge of whether individuals did or did not have COVID-19 infection.

Thirteen studies did not carry out testing as it would occur in practice: four studies used trained, centralised laboratory staff and not local laboratory or healthcare personnel; one test could not be purchased ([Diao 2020](#)); and 11 because the test was not conducted within the manufacturer instructions for use (these categories are not mutually exclusive). Four studies tested samples in a viral transport medium that was not covered by the manufacturer instructions for use, five used frozen samples, one reported heat inactivation of samples prior to direct testing and two reported a testing timeframe beyond that recommended.

The remaining five studies provided inadequate information to make a judgement; three of them did conduct the test within the manufacturer instructions for use but none of them clearly described the setting for testing or personnel conducting the test.

Reference standards

Only one study used an appropriate reference standard to define the presence or absence of COVID-19 infection (two negative PCR results required to confirm the absence of COVID-19) and implemented it in ways that prevented bias ([Diao 2020](#)). One

additional study reported two RT-PCR results for all study participants ([Moore 2020](#)), and two did not include non-COVID-19 cases. We considered that the remaining 14 did not use an adequate reference standard, putting them at high risk of bias ([Figure 2](#)). Eight studies reported blinded RT-PCR interpretation and 10 (56%) provided insufficient information about blinding of the reference standard to the index test to judge risk of bias.

RT-PCR is unlikely to falsely classify participants as having COVID-19 (low risk of false positive), but may miss true cases leading to false positives on the index test when a single RT-PCR alone is used as a reference standard. Four studies (22%) used a second RT-PCR test for samples with discrepant results (FP and FN) to address this. However, selective re-testing could miss additional cases of COVID-19 infection, and is likely to lead to distorted results. One study ([Moore 2020](#)), used a second RT-PCR test in all samples and furthermore carried out a record review for all cases with discrepant results in order to verify whether participants were truly considered to have had COVID-19 infection.

We judged 17 of the 18 studies to raise concerns for applicability (94%) because of defining the presence of COVID-19 infection based on a single RT-PCR-positive result. These studies will have excluded individuals who are RT-PCR-negative but have exposure and clinical features that meet the case definitions for COVID-19.

Flow and timing

Only three studies were at low risk of bias for participant flow and timing, one ([Porte 2020](#)), used a Standards of Reporting Diagnostic Accuracy Studies (STARD)-style participant flow diagram and checklist ([Bossuyt 2015](#)), to fully report outcomes for all samples. Five studies were at high risk of bias because of exclusion of samples following invalid index test results (they did not carry out any retesting).

Unclear risk of bias was present in 10 (56%) studies because of lack of clarity around participant inclusion and exclusion from analyses. Six studies were unclear regarding whether the analysis was participant-based or sample-based (where there is a possibility of multiple samples per participant overstating the precision of estimates).

Conflicts of interest

In six studies all authors declared no conflicts of interest, although one study that evaluated an 'in-house' test included a co-author affiliated to a test manufacturing company. Eight studies did not provide a conflict of interest statement (one of these included co-authors affiliated to the test manufacturer) and in the four remaining studies at least one author declared conflicts of interest in relation to the test.

Eleven studies provided no funding statement, five reported no funding sources to declare, and two reported one or more public funding sources. Two studies reported receipt of test kits or reagents 'in kind' from test manufacturers.

Findings

Of the 18 included studies, three reported evaluations of more than one test using the same samples ([Table 1](#)). In order to include all results from all tests in these analyses we have treated results from different tests of the same samples within a study as separate data points, such that data are available on 23 test evaluations

(8 evaluations of antigen tests in 5 studies and 15 evaluations of rapid molecular tests in 13 studies). The results table (Table 2), identifies where estimates are based on multiple assessments of the same samples by including both the number of test evaluations and the number of studies. The numbers of true positives, false positives, and total samples with and without confirmed SARS-CoV-2 infection are based on test result counts.

We undertook analyses separately for antigen tests and for molecular-based tests. We present results for all analyses in Table 2. Forest plots of study data for the primary analyses are in Figure 3 and Figure 4. Full identification details for all assays are provided in Appendix 8 and Appendix 9); for brevity, the antigen assays are referred to by the manufacturer name. Subgroup analyses according to viral load are in Figure 5 and Figure 6, and rapid molecular test results before and after discrepant analysis are in Figure 7.

Figure 3. Forest plot of studies evaluating antigen tests. Studies grouped by test (FIA: fluorescence immunoassays; CGIA: colloidal gold-based immunoassays; NP: nasopharyngeal; OP: oropharyngeal)

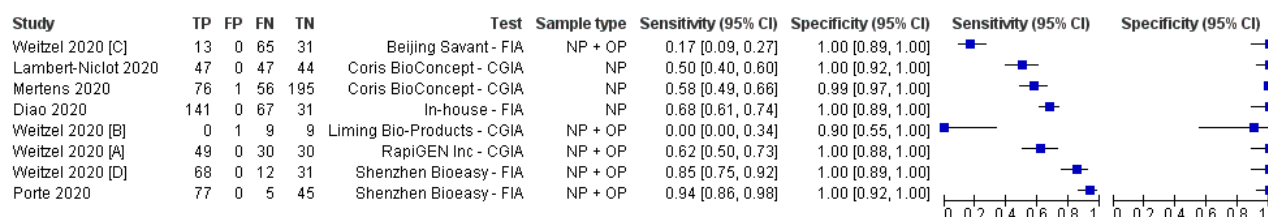


Figure 4. Forest plot of studies evaluating rapid molecular tests. Studies grouped by test and sample type (NP: nasopharyngeal; OP: oropharyngeal; RUO: research use only)


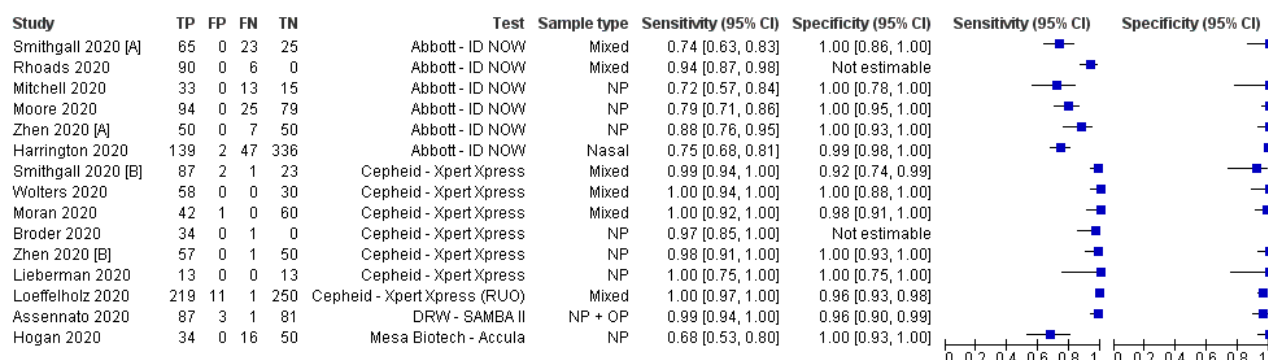


Figure 5. Forest plot of studies evaluating antigen tests according to viral load: high (≤ 25 Ct) versus low viral load (≤ 30 Ct in Diao 2020). Studies grouped by test

Antigen tests - high viral load

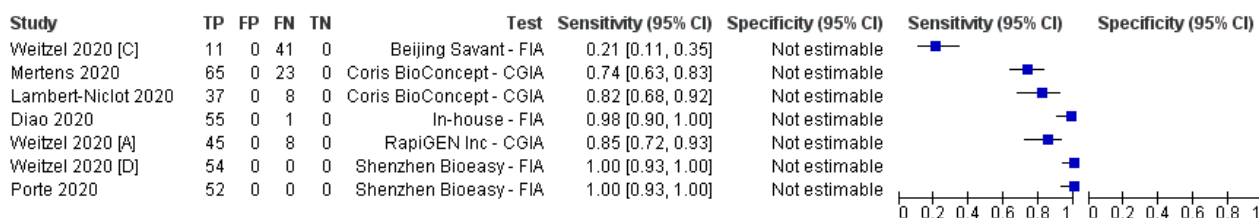

Antigen tests - low viral load


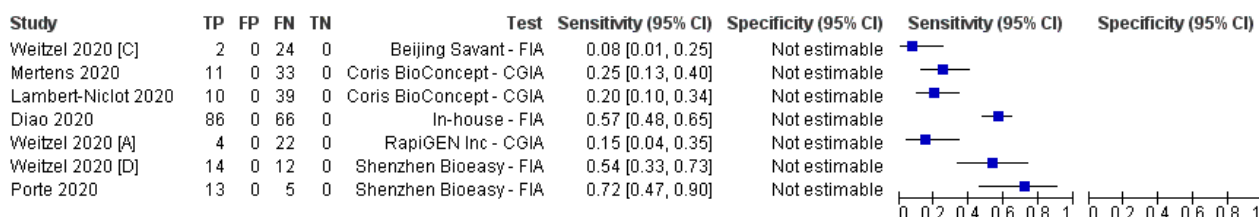


Figure 6. Forest plot of studies evaluating rapid molecular tests according to viral load: high (≤ 30 Ct) versus low viral load. Studies grouped by test

Molecular tests - high viral load

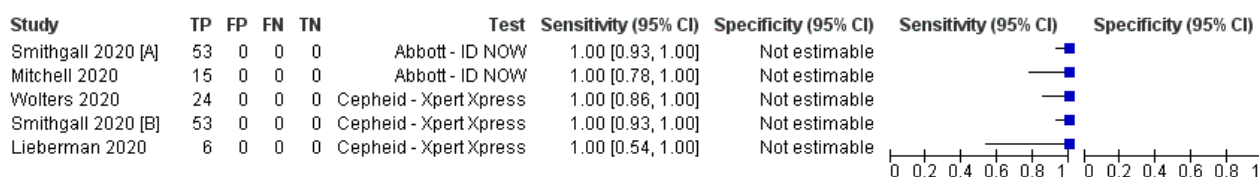

Molecular tests - low viral load

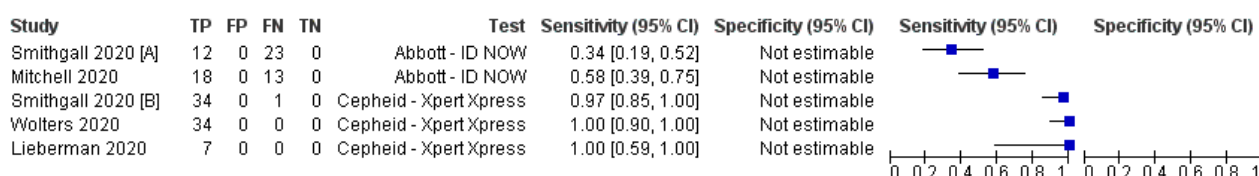


Figure 7. Forest plot of studies of molecular tests before and after discrepant analysis. Studies grouped by test (DRW: Diagnostics for the Real World; RUO: research use only)

Molecular tests - all (before discrepant analysis)

Study	TP	FP	FN	TN	Test	Sensitivity (95% CI)	Specificity (95% CI)	Sensitivity (95% CI)	Specificity (95% CI)
Harrington 2020	139	2	47	336	Abbott - ID NOW	0.75 [0.68, 0.81]	0.99 [0.98, 1.00]		
Assennato 2020	87	3	1	81	DRW - SAMBA II	0.99 [0.94, 1.00]	0.96 [0.90, 0.99]		
Loeffelholz 2020	219	11	1	250	Cepheid - Xpert Xpress (RUO)	1.00 [0.97, 1.00]	0.96 [0.93, 0.98]		
Moran 2020	42	1	0	60	Cepheid - Xpert Xpress	1.00 [0.92, 1.00]	0.98 [0.91, 1.00]		

Molecular tests - all (after discrepant analysis)

Study	TP	FP	FN	TN	Test	Sensitivity (95% CI)	Specificity (95% CI)	Sensitivity (95% CI)	Specificity (95% CI)
Harrington 2020	140	0	47	337	Abbott - ID NOW	0.75 [0.68, 0.81]	1.00 [0.99, 1.00]		
Assennato 2020	90	0	1	81	DRW - SAMBA II	0.99 [0.94, 1.00]	1.00 [0.96, 1.00]		
Moran 2020	42	0	0	61	Cepheid - Xpert Xpress	1.00 [0.92, 1.00]	1.00 [0.94, 1.00]		
Loeffelholz 2020	227	3	0	251	Cepheid - Xpert Xpress (RUO)	1.00 [0.98, 1.00]	0.99 [0.97, 1.00]		

Accuracy of antigen tests overall and by test

Average sensitivity across the eight evaluations of antigen tests was 56.2% (95% CI 29.5 to 79.8%), and average specificity 99.5% (95% CI 98.1% to 99.9%; 943 samples, including 596 samples with confirmed SARS-CoV-2; Table 2). However, Figure 3 shows considerable heterogeneity in sensitivity, with results across studies ranging from 0% to 94%. The average value should therefore be interpreted with caution as there may be real differences in sensitivity between the test brands. The two assays with lowest sensitivity (Liming Bio-Products and Beijing Savant assays) do not now appear to be commercially available. Pooled results for the two tests with two studies each suggested higher sensitivity for the Shenzhen Bioeasy FIA (89.5%, 95% CI 83.7% to 93.8%) than the Coris BioConcept CGIA (54.4%, 95% CI 47.7% to 61.0%), but these tests were not evaluated in the same studies and other factors may explain the observed differences. Similar, unknown factors may explain differences between the Shenzhen Bioeasy and Coris BioConcept assays and the other tests for which only single studies were available. Specificities were consistent and high, with point estimates of 99% or 100% in seven evaluations, and one study estimating specificity as 90% but with a 95% confidence interval that included 100%.

Accuracy of rapid molecular tests overall and by test

Average sensitivity and specificity for the 13 rapid molecular test evaluations that included samples with and without SARS-CoV-2, were 95.2% (95% CI 86.7% to 98.3%) and 98.9% (95% CI 97.3% to 99.5%; 2255 samples, 1179 with confirmed SARS-CoV-2). Adding the two 'cases only' studies made little difference to the average sensitivity (95.5%, 95% CI 88.5% to 98.4%; 1244 cases). We excluded these two studies from further analyses (Broder 2020; Rhoads 2020).

Figure 4 demonstrates heterogeneity in sensitivity estimates (ranging from 68% to 100%), with consistently high specificities (92% to 100%, but with upper limits of 95% CIs of 99% or 100% in every study). Of the four different molecular tests evaluated, two were evaluated in one study each. The sensitivity and specificity of the Accula test were 68.0% (95% CI 53.3% to 80.5%) and 100% (95% CI 92.9% to 100%; 100 samples, 50 with confirmed SARS-CoV-2). For SAMBA II, sensitivity and specificity were 98.9% (95% CI 93.8% to

100%) and 96.4% (95% CI 89.9% to 99.3%; 172 samples, 88 with confirmed SARS-CoV-2).

The ID NOW and Xpert Xpress tests were evaluated in five studies (1003 samples, 496 with confirmed SARS-CoV-2) and six studies (919 samples, 479 with confirmed SARS-CoV-2), respectively. Pooled analysis showed the Xpert Xpress test to have higher sensitivity (99.4%, 95% CI 98.0% to 99.8%) in comparison to ID NOW (76.8%, 95% CI 72.9% to 80.3%), a difference of 22.6 (95% CI 18.8 to 26.3) percentage points (Table 2). Whilst the specificity of Xpert Xpress (96.8%, 95% CI 90.6% to 99.0%) was marginally lower than ID-NOW (99.6%, 95% CI 98.4% to 99.9%) the difference was of a magnitude that can be explained by chance (difference of -2.8, 95% CI -6.4 to 0.8) percentage points ($P = 0.13$). Restricting the analysis to the two studies that compared the two tests in the same patients gave very similar results (difference in sensitivity of 19.3% (95% CI 12.5% to 26.2%) and difference in specificity of -2.7 percentage points (95% CI -6.3 to 1.0), based on 221 samples, 146 with SARS-CoV-2; Smithgall 2020 [A]; Zhen 2020 [A])). (This analysis used the two-sample test of proportions).

Subgroup analyses by sample type

Adequate data for different sample types were available for studies using nasopharyngeal samples only. We observed similar average sensitivity (59.4%, 95% CI 50.7% to 67.5%) and specificity (99.6%, 95% CI 97.4% to 99.9%) for three evaluations of antigen tests (705 samples, 434 with confirmed SARS-CoV-2). For six evaluations of molecular tests, average sensitivity appeared lower compared to the overall pooled estimate (87.1%, 95% CI 71.6% to 94.7%) with little change in specificity (Table 2).

Subgroup analyses by viral load

We extracted sensitivity data according to viral load from seven evaluations of antigen tests (three with the assistance of the study authors) and five evaluations of molecular tests. Ct threshold for high viral load was 25 or less for four of the five antigen studies and 30 or less for the remaining antigen evaluation and for all of the molecular assay evaluations. We observed a large difference in sensitivity in the high viral load group (400 with confirmed SARS-CoV-2) for antigen tests (difference of 60.6 percentage points (95% CI 38.2, 83.0) compared to low viral load (341 samples with

confirmed SARS-CoV-2) that was beyond that expected by chance ($P < 0.001$) (Table 2; Figure 5).

For molecular tests, all sensitivity estimates for the high viral load subgroups were 100% (based on 151 samples with confirmed SARS-CoV-2) compared to between 34% and 100% for low viral load subgroups (summary sensitivity 93.3%, 95% CI 46.7% to 99.6%; 142 samples with confirmed SARS-CoV-2; Table 2; Figure 6). The evaluations with the lowest sensitivities both evaluated ID NOW, with reported sensitivity estimates of 34% (35 samples with confirmed SARS-CoV-2 in Smithgall 2020 [A]), and 58% (based on 31 samples with confirmed SARS-CoV-2 in Mitchell 2020). Sensitivity in the three evaluations of Xpert Xpress ranged from 97% (35 samples with confirmed SARS-CoV-2 in Smithgall 2020 [B]) to 100% (in Lieberman 2020 and Wolters 2020, with 7 and 34 samples with confirmed SARS-CoV-2 respectively).

Sensitivity analysis of the impact of discrepant analysis

Four evaluations of molecular tests (in 1566 samples) reported results before and after discrepant analysis where selected samples were re-tested with either the same (Harrington 2020; Moran 2020), or an alternative RT-PCR assay (Assennato 2020; Loeffelholz 2020), three of which also reported re-testing of samples with the index test (Assennato 2020; Harrington 2020; Moran 2020; Table 3; Figure 7).

Discrepant analysis always works to reduce the number of samples deemed to be false negative or false positive errors. Discrepant analysis reduced the false negative proportion (1-sensitivity) from 1.8% to 0.5% and the false positive rate (1-specificity) from 2.2% to 0.4%. Three of the four studies reporting initially 'false positive' results reported zero false positives after sample re-testing and one reported a drop in false positives from 11 to 3 (Loeffelholz 2020; Table 3). One of the two studies reporting re-testing of initially 'false negative' results reported reclassification as true negative on re-testing, and in the other the false negative remained as a false negative. Given the bias inherent in choosing the reference test dependent on the observed results, we caution against these findings.

An additional study tested all samples with two different RT-PCR assays, and hence used a more accurate reference standard in all samples, not just samples with discrepant results (Moore 2020), in which six initial true negatives were reclassified as false negatives after the second RT-PCR. Had discrepant analysis been undertaken these misclassifications would have been missed, further underlining the methodological flaws inherent to discrepant analysis.

Other sources of heterogeneity

We planned to evaluate the effect of other sources of heterogeneity, including study design, reference standard, length and severity of symptoms, and setting. However, additional formal investigations using meta-regression were not possible because of limited data, lack of reporting or lack of variability across the studies in these features (Appendix 11). Only one study reported the median time to testing after symptom onset, none reported symptom severity, and three reported the setting in which tests were conducted. All studies used RT-PCR alone as the reference standard for diagnosing COVID-19 infection.

We anticipate revisiting the effect of study design and including a more detailed investigation by sample type in future iterations of this review.

DISCUSSION

This is the first version of a Cochrane living review summarising the accuracy of point-of-care antigen and molecular tests for detecting current SARS-CoV-2 infection. This version of the review is based on published studies, or studies available as preprints, up until 25 May 2020. We are continually identifying new published studies, and plan regular updates of this review.

Summary of main results

We included data from 18 studies including 3198 samples (including 1775 samples with confirmed SARS-CoV-2). Five studies, reporting eight test evaluations, considered antigen tests and 13 studies, reporting 15 test evaluations, considered rapid molecular tests. Key findings are presented in the Summary of findings 1.

We summarise five key findings from this review.

1. A significant proportion of antigen and molecular assays that are suitable for use at the point of care do not have any published or preprint reports of accuracy. This review has evaluated data from five commercial antigen tests, two of which we could not identify as available for purchase, and four molecular assays. These represent a small proportion of assays currently available. We have identified 24 additional studies of rapid antigen or molecular tests published or available as preprints up until 22 June 2020, which we will appraise for inclusion in the review update, but there still remain no published data for the majority of tests on the current FIND list.
2. The design and execution of studies limits the strength of conclusions that we are currently able to draw, either for antigen or for molecular tests. It is unclear whether the limitations in the primary studies will lead to over- or under-estimates of test accuracy, thus all results we report should be interpreted with a high degree of caution. Half of studies used deliberate sampling based on the presence or absence of confirmed COVID-19 infection, and the majority selected samples from those submitted to laboratories for routine RT-PCR testing with little to no detail of the participants who provided the samples in relation to either symptom status or time from symptom onset. It is impossible to determine the effect of inclusion decisions based on the availability of residual or remnant samples. It was not always clear how many samples were included from each participant, and the analysis had to be undertaken on a per-sample basis, which will have overestimated the precision of the estimates. RT-PCR was the only reference standard for diagnosing the presence of SARS-CoV-2 infection so that we are unable to comment on the accuracy of rapid tests for diagnosing infection in those who are RT-PCR negative but meet case definition criteria for the presence of infection. The use of a second RT-PCR assay to determine the disease status of samples with discrepant results following rapid molecular testing is likely to introduce further bias.
3. Three-quarters of studies conducted tests outside of manufacturers' instructions for use, particularly in regard to sample storage and use of transport media, and with tests conducted in centralised laboratories rather than at the point of care, so that test accuracy in a clinical setting remains

unknown. We considered five tests, including one molecular assay, to have low complexity in terms of minimal sample preparation and test steps, and the other four to have moderate ($n = 3$) or high ($n = 1$) complexity, which could also affect how well the observed accuracy translates into practice. We did not include interpretation steps in our assessment of test complexity; however the use of reader devices, for example for FIAs, could be considered to further add to complexity.

4. On average, the sensitivity of antigen tests was relatively poor (56.2%, 95% CI 29.5 to 79.8%), but with consistently high specificities (average 99.5%, 95% CI 98.1 to 99.9%). However, there is considerable heterogeneity in sensitivities between studies, and with limited data for individual tests. We observed large differences in sensitivity according to viral load and suspect that differences in the distribution of samples with high and low viral load between studies may have affected overall accuracy estimates. Combined with methodological limitations and other unknown factors, it is not possible to state with any certainty whether any test is superior to the others. There is a suggestion of higher sensitivity in two studies of the Shenzhen Bioeasy fluorescent immunoassay (sensitivity 89.5%, 95% CI 83.8%, 93.3%), that was maintained in subgroup analysis by viral load (one of the two obtained over 90% of samples during the first week of symptoms). An additional study reporting the development of this assay reported lower sensitivity overall (68%, 95% CI 61, 74%), however it included a much lower proportion of samples with high viral load (27% compared to 68 to 74% in the other two studies). Subgroup analysis suggested the test performed similarly to the other two studies when restricted to high and low viral load subgroups. All three studies included high percentages of samples with confirmed SARS-CoV-2, and more data is needed to determine whether test performance for this assay can be repeated in clinical practice.
5. On average, the sensitivity for the rapid molecular tests was 95.2% (95%CI 86.7%, 98.3%) with specificity 98.9% (95% CI 97.3, 99.5%). Although the average estimates are based on twice as much data as for the antigen tests, the evaluations are subject to the same methodological limitations, and we do not know how the assays would perform in any specific clinical setting when used in people suspected of having COVID-19 infection or of having been exposed to a confirmed case.

Most of the evaluations of molecular tests were of ID NOW or Xpert Xpress. Summary sensitivity for Xpert Xpress (99.4%, 95% CI 98.0 to 99.8%) was 22.6 percentage points higher than that of ID NOW, a magnitude of difference that was more or less maintained in the two direct comparisons of the two assays. Concerns over risk of bias would suggest that this high rate of sensitivity might be an over-estimate. However as both sets of studies have similar methodological limitations, it is probably reasonable to presume that some difference in sensitivity between tests would be maintained if these sources of bias were removed. The difference in specificity between the tests is small (ID NOW being 2.8% more specific compared to Xpert Xpress), but potentially important especially if used in a low-prevalence setting. However, this would not be an issue should test positives be confirmed by a laboratory-based RT-PCR assay. Concerns about the applicability of study participants and index tests brings into question whether similar differences in test performance would be observed in practice.

As stated above, we did not undertake a formal comparison between antigen and molecular assays because of the lack of

direct head-to-head comparisons of the two test types. However, the possible effect of the observed differences in accuracy can be illustrated by applying the summary estimates of test accuracy to a hypothetical cohort of 1000 people suspected of COVID-19 infection ([Summary of findings 1](#)). If 100 people had confirmed SARS-CoV-2 infection (prevalence of 10%), the average sensitivity and specificities of antigen tests mean that 5 of 61 people with a positive test result would be false positives (positive predictive value (PPV) 92%) while 44 of 940 people with negative test results would be falsely negative (negative predictive value (NPV) 95%). As there is high heterogeneity in the estimates of sensitivity, the values observed in practice could vary considerably from these figures. For molecular assays at the same prevalence, 10 of 105 positive test results would be false positive (PPV 90%), and 5 of 895 with negative results would be falsely negative (NPV 99%).

Small decreases (to 5%) or increases (to 20%) in prevalence make little difference to the absolute number of false positive results, but have a large relative effect when considered in relation to the number of positive test results (PPV ranging 85% to 97% for antigen tests and 83% to 95% for molecular assays). The NPV (percentage of negative test results that are truly negative) for the molecular assays is not affected by these prevalence changes in the same way because of the relatively high sensitivity and relatively low-prevalence scenarios considered. Wider variation is observed for antigen tests (98% to 90%). This shows how even in a low-prevalence setting, tests with poor sensitivity can have a considerable impact on the level of confidence that can be had in a negative test result. However, we emphasise that these numbers are not based on any evidence comparing antigen and molecular tests in the same samples.

We saw a similar pattern of results when applying summary results for individual tests with wide variations in sensitivity and only small differences in specificities ([Summary of findings 1](#)).

Strengths and weaknesses of the review

Our review used a broad search screening all articles concerning COVID-19. We undertook all screening and eligibility assessments, QUADAS-2 assessments ([Whiting 2011](#)), and data extraction of study findings independently and in duplicate. Whilst we have reasonable confidence in the completeness and accuracy of the findings up until the search date, should errors be noted please inform us at covidtda@contacts.bham.ac.uk so that we can check and correct in our next update.

We identified one other systematic review of point-of-care tests for detection of SARS-CoV-2 that is currently available only as a preprint ([Subsoontorn 2020](#)). The review did not consider antigen tests or RT-PCR-based tests (such as Xpert Xpress), instead focusing on molecular tests that do not require the use of a thermal cycler. We undertook a careful assessment of test complexity to ensure that included tests were suitable for use at the point of care. This assessment included explicit consideration of sample preparation and biosafety requirements as well as time to test result. The application of these index test criteria led to the exclusion of the majority of the 31 RT-LAMP or CRISPr assay evaluations that were included in [Subsoontorn 2020](#). Evaluations of alternative laboratory-based molecular technologies are under consideration for inclusion in another review in our series of Cochrane COVID-19 DTA reviews. An additional seven studies included in [Subsoontorn](#)

2020 became available after our search cut-off and are already under consideration for inclusion in the review update.

Weaknesses of the review primarily reflect the weaknesses in the primary studies and their reporting. Many studies omitted descriptions of participants, and key aspects of study design and execution. In order to include data for all tests in pooled analyses we have had to include some samples multiple times. We have been explicit about these issues where they arose. It is possible that eligible studies have been missed by our search strategy however we believe the risk to be very low considering our broad approach to identification of literature.

Around a quarter (5/18) of the studies we have included are currently only available as preprints, and as yet, have not undergone peer review. As published versions of these studies are identified in the future, we will double-check study descriptions, methods and findings, and update the review as required.

Applicability of findings to the review question

We have concerns about the applicability of the evidence that we have identified for point-of-care tests.

Due to lack of reporting, we do not know whether tests perform in the same way or differently according to whether those being tested have symptoms of COVID-19, and if so how long they have experienced those symptoms for, or are asymptomatic. Studies appeared to include remnant or residual samples for testing and many selectively included high percentages of samples with RT-PCR-confirmed SARS-CoV-2. In reality, point-of-care tests will be considered for use in much lower prevalence settings. Methodological work on diagnostic test evaluations has shown that independently of prevalence, tests do not necessarily exhibit the same sensitivity and specificity in different prevalence settings (Usher-Smith 2016). This can be because of differences in the case-mix or 'spectrum' of disease (e.g. viral load). However, the mechanisms in action can be complex and difficult to clearly identify (Leeflang 2013).

We also had concerns about the way in which many of the tests evaluated were performed outside of manufacturer instructions for use, and not in fact at the point of care.

Great caution should be taken in applying these results outside of the individual study contexts.

AUTHORS' CONCLUSIONS

Implications for practice

In the [Role of index test\(s\)](#) section, we suggested two main roles for point-of-care testing.

1. As a replacement for laboratory-based RT-PCR, if sufficiently accurate. Evidence included to date suggests that some rapid molecular tests might have accuracy levels approximating those of laboratory-based RT-PCR. However, many of the data come from two-group studies with deliberate over-sampling of cases and concerns over the applicability of the evidence. We cannot be certain as to whether any test performs sufficiently well for this role.
2. As a triage to RT-PCR, allowing earlier detection and rapid management (self-isolation, quarantine or therapeutic

intervention) of those testing positive; those with negative results waiting for the laboratory-based RT-PCR result. On current evidence of test performance (using average observed sensitivities and specificities), rapid tests could only perform this type of triage role in higher-prevalence settings (i.e. 20% or higher) because of the (relative) risk of false positive results in lower-prevalence settings. Although average test specificities are high for both antigen and for molecular tests, unnecessary quarantine measures for 1 in 6 (83% PPV), or even 1 in 10 (90% PPV), people with a positive test result would seem a relatively high price to pay for a rapid result. The 99% to 100% specificities observed for individual tests would need to be replicated in well designed field studies, and following manufacturers' instructions for use, before any test could be recommended for use as a triage test.

Alternatively, serial testing (over a number of days), or combinations of different rapid tests (e.g. an antigen test followed by a rapid molecular test) on the same sample may provide a useful testing strategy; however, additional evidence of the performance of any such diagnostic strategy would be needed. In the absence of further evidence, and in low prevalence settings, both positive and negative results from any of the rapid point-of-care tests included in this review would need to be followed up with a laboratory-based RT-PCR.

Ultimately, decisions around rapid testing will be driven not only by diagnostic accuracy but by acceptable levels of test complexity, time to result, and acceptability to those being tested, all of which might vary according to the setting in which the tests are to be used. In settings where RT-PCR is not available, rapid tests may have a role if acceptable performance targets for diagnostic test accuracy, such as those laid out in WHO's priority target product profiles for COVID-19 diagnostics, can be met (WHO 2020c).

Implications for research

A considerable volume of research has already emerged for point-of-care tests for COVID-19 infection. However further prospective and comparative evaluations of individual tests, either alone or in combination, and in clinically relevant settings are urgently needed. These settings include those where people with signs and symptoms present for testing as well as those involving testing asymptomatic people who may have come into contact with confirmed cases. Reliable and ideally rapid diagnostic tests are the keystone to good track and trace programmes, as a means of implementing necessary self-isolation or quarantine and reducing community transmission. Studies should recruit consecutive series of eligible participants and should clearly describe symptomatic status, and should document time from symptom onset or time since exposure. Point-of-care tests must be conducted in accordance with manufacturer instructions for use, and across the spectrum of point-of-care settings and test operators.

We observed a number of studies of molecular assays employing discrepant analysis to confirm the disease status of samples with false positive results in particular. There is a considerable risk of this type of selective re-testing leading to distorted results. If there is sufficient concern about the reliability of a single RT-PCR test then all samples should be tested with two RT-PCR assays. Finally, any future research study needs to be clear about eligibility and exclusion decisions throughout the whole diagnostic pathway,

and should conform to the updated Standards for Reporting of Diagnostic Accuracy (STARD) guideline ([Bossuyt 2015](#)).

ACKNOWLEDGEMENTS

Members of the Cochrane COVID-19 Diagnostic Test Accuracy Review Group include:

- the project team (Deeks JJ, Dinnes J, Takwoingi Y, Davenport C, Leeftang MMG, Spijker R, Hooft L, Van den Bruel A, McInnes MDF, Emperador D, Dittrich S, Cunningham J);
- the systematic review teams for each review:
 - * Molecular, antigen, and antibody tests (Adriano A, Beese S, Dretzke J, Ferrante di Ruffano L, Harris I, Price M, Taylor-Phillips S)
 - * Signs and symptoms (Stuyf T, Domen J, Horn S)
 - * Routine laboratory markers (Yang B, Langendam M, Ochodo E, Guleid F, Holtman G, Verbakel J, Wang J, Stegeman I)
 - * Imaging tests (Salameh JP, McGrath TA, van der Pol CB, Frank RA, Prager R, Hare SS, Dennie C, Jenniskens K, Korevaar DA, Cohen JF, van de Wijgert J, Damen JAAG, Wang J);
- the wider team of systematic reviewers from University of Birmingham, UK who assisted with title and abstract screening across the entire suite of reviews for the diagnosis of COVID-19 (Agarwal R, Baldwin S, Berhane S, Herd C, Kristunas C, Quinn L, Scholefield B).

The editorial process for this review was managed by Cochrane's EMD Editorial Service in collaboration with Cochrane Infectious Diseases. We thank Helen Wakeford, Anne-Marie Stephani and Deirdre Walshe for their comments and editorial management. We

thank Sarah Hodgkinson for comments on the Abstract. We thank Robin Featherstone and Douglas M Salzwedel for comments on the search and Mike Brown and Paul Garner for sign-off comments. We thank Denise Mitchell for her efforts in copy-editing this review.

Thank you also to peer referees Kristien Verdonck, Tivani Mashamba-Thompson, Fergus Macbeth, consumer referee Brian Duncan and methodological referees Mia Schmidt-Hansen and Jo Leonardi-Bee, for their insights.

The editorial base of Cochrane Infectious Diseases is funded by UK aid from the UK Government for the benefit of low- and middle-income countries (project number 300342-104). The views expressed do not necessarily reflect the UK Government's official policies.

The authors thank Dr Mia Schmidt-Hansen who was the Cochrane Diagnostic Test Accuracy (DTA) Contact Editor for this review; the clinical and methodological referees; the Cochrane DTA Editorial Team; and Anne Lawson who copy-edited the protocol.

Jonathan Deeks is a UK National Institute for Health Research (NIHR) Senior Investigator Emeritus. Yemisi Takwoingi is supported by a NIHR Postdoctoral Fellowship. Jonathan Deeks, Jacqueline Dinnes, Yemisi Takwoingi, Clare Davenport and Malcolm Price are supported by the NIHR Birmingham Biomedical Research Centre. This paper presents independent research supported by the NIHR Birmingham Biomedical Research Centre at the University Hospitals Birmingham NHS Foundation Trust and the University of Birmingham. The views expressed are those of the author(s) and not necessarily those of the NHS, the NIHR or the Department of Health and Social Care.

REFERENCES

References to studies included in this review

Assennato 2020 {published data only}

only} [10.1101/2020.05.24.20100990](https://doi.org/10.1101/2020.05.24.20100990)

Assennato SM, Ritchie AV, Nadala C, Goel N, Zhang H, Datir R, et al. Performance evaluation of the point-of-care SAMBA II SARS-CoV-2 test for detection of SARS-CoV-2. *medRxiv [Preprint]* 24 May 2020. [DOI: [10.1101/2020.05.24.20100990](https://doi.org/10.1101/2020.05.24.20100990)]

Broder 2020 {published data only}

* Broder K, Babiker A, Myers C, White T, Jones H, Cardella J, et al. Test agreement between Roche cobas 6800 and Cepheid GeneXpert Xpress SARS-CoV-2 assays at high cycle threshold ranges. *Journal of Clinical Microbiology* 2020;**58**:e01187-20. [DOI: [10.1128/JCM.01187-20](https://doi.org/10.1128/JCM.01187-20)]

Broder KJ, Babiker A, Myers C, White T, Jones H, Cardella J, et al. Test agreement between Roche cobas 6800 and Cepheid GeneXpert Xpress SARS-CoV-2 assays at high cycle threshold ranges. *bioRxiv [Preprint]* 5 May 2020:1-13. [DOI: [10.1101/2020.05.05.078501](https://doi.org/10.1101/2020.05.05.078501)]

Diao 2020 {published data only}

Diao B, Wen K, Chen J, Liu Y, Yuan Z, Han C, et al. Diagnosis of acute respiratory syndrome coronavirus 2 infection by detection of nucleocapsid protein. *medRxiv [Preprint]* 10 March 2020:1-13. [DOI: [10.1101/2020.03.07.20032524](https://doi.org/10.1101/2020.03.07.20032524)]

Harrington 2020 {published data only}

Harrington A, Cox B, Snowdon J, Bakst J, Ley E, Grajales P, et al. Comparison of Abbott ID NOW and Abbott m2000 methods for the detection of SARS-CoV-2 from nasopharyngeal and nasal swabs from symptomatic patients. *Journal of Clinical Microbiology* 2020;**58**(8):e00798-20. [DOI: [10.1128/JCM.00798-20](https://doi.org/10.1128/JCM.00798-20)]

Hogan 2020 {published data only}

Hogan CA, Garamani N, Lee AS, Tung JK, Sahoo MK, Huang C, et al. Comparison of the Accula SARS-CoV-2 test with a laboratory-developed assay for detection of SARS-CoV-2 RNA in clinical nasopharyngeal specimens. *bioRxiv [Preprint]* 2020. [DOI: [10.1101/2020.05.12.092379v1](https://doi.org/10.1101/2020.05.12.092379v1)]

Lambert-Niclot 2020 {published data only}

Lambert-Niclot S, Cuffel A, Le Pape S, Vauloup-Fellous C, Morand-Joubert L, Roque-Afonso AM, et al. Evaluation of a rapid diagnostic assay for detection of SARS-CoV-2 antigen in nasopharyngeal swab. *Journal of Clinical Microbiology* 2020;**58**(8):e00977-20. [DOI: [10.1128/JCM.00977-20](https://doi.org/10.1128/JCM.00977-20)]

Lieberman 2020 {published data only}

Lieberman JA, Pepper G, Naccache SN, Huang ML, Jerome KR, Greninger AL. Comparison of commercially available and laboratory developed assays for in vitro detection of SARS-CoV-2 in clinical laboratories. *Journal of Clinical Microbiology* 2020;**58**(8):e00821-20. [DOI: [10.1128/JCM.00821-20](https://doi.org/10.1128/JCM.00821-20)]

Loeffelholz 2020 {published data only}

Loeffelholz MJ, Alland D, Butler-Wu SM, Pandey U, Perno CF, Nava A, et al. Multicenter evaluation of the Cepheid Xpert Xpress SARS-CoV-2 test. *Journal of Clinical Microbiology* 2020;**58**(8):e00926-20. [DOI: [10.1128/JCM.00926-20](https://doi.org/10.1128/JCM.00926-20)]

Mertens 2020 {published data only}

Mertens P, De Vos N, Martiny D, Jassoy C, Mirazimi A, Cuypers L, et al. Development and potential usefulness of the COVID-19 Ag Respi-Strip diagnostic assay in a pandemic context. *medRxiv [Preprint]* 24 April 2020:1-29. [DOI: [10.1101/2020.04.24.20077776](https://doi.org/10.1101/2020.04.24.20077776)]

Mitchell 2020 {published data only}

Mitchell SL, George KS. Evaluation of the COVID19 ID NOW EUA assay. *Journal of Clinical Virology* 2020;**128**:104429. [DOI: [10.1016/j.jcv.2020.104429](https://doi.org/10.1016/j.jcv.2020.104429)]

Moore 2020 {published data only}

Moore NM, Li H, Schejbal D, Lindsley J, Hayden M. Comparison of two commercial molecular tests and a laboratory-developed modification of the CDC 2019-nCoV RT-PCR assay for the qualitative detection of SARS-CoV-2 from upper respiratory tract specimens. *medRxiv [Preprint]* 2020:1-22. [DOI: [10.1101/2020.05.02.20088740](https://doi.org/10.1101/2020.05.02.20088740)]

Moran 2020 {published data only}

Moran A, Beavis KG, Matushek SM, Ciaglia C, Francois N, Tesic V, et al. The detection of SARS-CoV-2 using the Cepheid Xpert Xpress SARS-CoV-2 and Roche cobas SARS-CoV-2 assays. *Journal of Clinical Microbiology* 2020;**58**(8):e00772-20. [DOI: [10.1128/JCM.00772-20](https://doi.org/10.1128/JCM.00772-20)]

Porte 2020 {published data only}

Porte L, Legarraga P, Vollrath V, Aguilera X, Munita JM, Araos R, et al. Evaluation of novel antigen-based rapid detection test for the diagnosis of SARS-CoV-2 in respiratory samples. *papers.ssrn.com/abstract=3569871* 14 April 2020:1-23.

Rhoads 2020 {published data only}

Rhoads DD, Cherian SS, Roman K, Stempak LM, Schmotzer CL, Sadri N. Comparison of Abbott ID NOW, Diasorin Simplexa, and CDC FDA EUA methods for the detection of SARS-CoV-2 from nasopharyngeal and nasal swabs from individuals diagnosed with COVID-19. *Journal of Clinical Microbiology* 2020;**58**(8):e00760-20. [DOI: [10.1128/JCM.00760-20](https://doi.org/10.1128/JCM.00760-20)]

Smithgall 2020 [A] {published data only}

Smithgall MC, Scherberkova I, Whittier S, Green D. Comparison of Cepheid Xpert Xpress and Abbott ID Now to Roche cobas for the rapid detection of SARS-CoV-2. *bioRxiv [Preprint]* 25 April 2020:1-16. [DOI: [10.1101/2020.04.22.055327](https://doi.org/10.1101/2020.04.22.055327)]

* Smithgall MC, Scherberkova I, Whittier S, Green DA. Comparison of Cepheid Xpert Xpress and Abbott ID Now to Roche Cobas for the rapid detection of SARS-CoV-2. *Journal of Clinical Virology* 2020;**128**:104428. [DOI: [10.1016/j.jcv.2020.104428](https://doi.org/10.1016/j.jcv.2020.104428)]

Smithgall 2020 [B] {published data only}

Smithgall MC, Scherbergova I, Whittier S, Green DA. Comparison of Cepheid Xpert Xpress and Abbott ID Now to Roche Cobas for the rapid detection of SARS-CoV-2. *Journal of Clinical Virology* 2020;**128**:104428. [DOI: [10.1016/j.jcv.2020.104428](https://doi.org/10.1016/j.jcv.2020.104428)]

Weitzel 2020 [A] {published data only}

Weitzel T, Legarraga P, Iruretagoyena M, Pizarro G, Vollrath V, Araos R, et al. Head-to-head comparison of four antigen-based rapid detection tests for the diagnosis of SARS-CoV-2 in respiratory samples. *bioRxiv [Preprint]* 30 May 2020:1-21. [DOI: [10.1101/2020.05.27.119255](https://doi.org/10.1101/2020.05.27.119255)]

Weitzel 2020 [B] {published data only}

Weitzel T, Legarraga P, Iruretagoyena M, Pizarro G, Vollrath V, Araos R, et al. Head-to-head comparison of four antigen-based rapid detection tests for the diagnosis of SARS-CoV-2 in respiratory samples. *bioRxiv [Preprint]* 30 May 2020:1-21. [DOI: [10.1101/2020.05.27.119255](https://doi.org/10.1101/2020.05.27.119255)]

Weitzel 2020 [C] {published data only}

Weitzel T, Legarraga P, Iruretagoyena M, Pizarro G, Vollrath V, Araos R, et al. Head-to-head comparison of four antigen-based rapid detection tests for the diagnosis of SARS-CoV-2 in respiratory samples. *bioRxiv [Preprint]* 30 May 2020:1-21. [DOI: [10.1101/2020.05.27.119255](https://doi.org/10.1101/2020.05.27.119255)]

Weitzel 2020 [D] {published data only}

Weitzel T, Legarraga P, Iruretagoyena M, Pizarro G, Vollrath V, Araos R, et al. Head-to-head comparison of four antigen-based rapid detection tests for the diagnosis of SARS-CoV-2 in respiratory samples. *bioRxiv [Preprint]* 30 May 2020:1-21. [DOI: [10.1101/2020.05.27.119255](https://doi.org/10.1101/2020.05.27.119255)]

Wolters 2020 {published data only}

Wolters F, Van de Bovenkamp J, Van den Bosch B, Van den Brink S, Broeders M, Chung NH, et al. Multi-center evaluation of Cepheid Xpert(R) Xpress SARS-CoV-2 point-of-care test during the SARS-CoV-2 pandemic. *Journal of Clinical Virology* 2020;**128**:104426. [DOI: [10.1016/j.jcv.2020.104426](https://doi.org/10.1016/j.jcv.2020.104426)]

Zhen 2020 [A] {published data only}

Zhen W, Smith E, Manji R, Schron D, Berry GJ. Clinical evaluation of three sample-to-answer platforms for the detection of SARS-CoV-2. *Journal of Clinical Microbiology* 2020;**58**(8):e00783-20. [DOI: [10.1128/JCM.00783-20](https://doi.org/10.1128/JCM.00783-20)]

Zhen 2020 [B] {published data only}

Zhen W, Smith E, Manji R, Schron D, Berry GJ. Clinical evaluation of three sample-to-answer platforms for the detection of SARS-CoV-2. *Journal of Clinical Microbiology* 2020;**58**(8):e00783-20. [DOI: [10.1128/JCM.00783-20](https://doi.org/10.1128/JCM.00783-20)]

References to studies excluded from this review
Ai 2020 {published data only}

Ai JW, Zhang HC, Xu T, Wu J, Zhu M, Yu YQ, et al. Optimizing diagnostic strategy for novel coronavirus pneumonia, a multi-center study in Eastern China. *medRxiv [Preprint]* 17 February 2020:1-18. [DOI: [10.1101/2020.02.13.20022673](https://doi.org/10.1101/2020.02.13.20022673)]

Anahtar 2020 {published data only}

Anahtar MN, McGrath GE, Rabe BA, Tanner NA, White BA, Lennerz JK, et al. Clinical assessment and validation of a rapid and sensitive SARS-CoV-2 test using reverse-transcription loop-mediated isothermal amplification. *medRxiv [Preprint]* 18 May 2020:1-22. [DOI: [10.1101/2020.05.12.20095638](https://doi.org/10.1101/2020.05.12.20095638)]

Arumugam 2020 {published data only}

Arumugam A, Faron ML, Yu P, Markham C, Wong S. A rapid COVID-19 RT-PCR detection assay for low resource settings. *bioRxiv [Preprint]* 30 April 2020:1-13. [DOI: [10.1101/2020.04.29.069591](https://doi.org/10.1101/2020.04.29.069591)]

Baek 2020 {published data only}

Baek YH, Um J, Antigua KJ, Park JH, Kim Y, Oh S, et al. Development of a reverse transcription-loop-mediated isothermal amplification as a rapid early-detection method for novel SARS-CoV-2. *Emerging Microbes & Infections* 2020;**9**(1):998-1007.

Barra 2020 {published data only}

Barra GB, Ticiane Henriques SR, Goes MP, Henriques JR, Nery LF. Analytical sensibility and specificity of two RT-qPCR protocols for SARS-CoV-2 detection performed in an automated workflow. *medRxiv [Preprint]* 10 March 2020:1-5. [DOI: [10.1101/2020.03.07.20032326](https://doi.org/10.1101/2020.03.07.20032326)]

Basu 2020 {published data only}

Basu A, Zinger T, Inglima K, Woo KM, Atie O, Yurasits L, et al. Performance of Abbott ID NOW COVID-19 rapid nucleic acid amplification test in nasopharyngeal swabs transported in viral media and dry nasal swabs, in a New York City academic institution. *Journal of Clinical Microbiology* 2020;**58**(8):e01136-20. [DOI: [10.1128/JCM.01136-20](https://doi.org/10.1128/JCM.01136-20)]

Behrmann 2020 {published data only}

Behrmann O, Bachmann I, Spiegel M, Schramm M, El Wahed AA, Dobler G, et al. Rapid detection of SARS-CoV-2 by low volume real-time single tube reverse transcription recombinase polymerase amplification using an exo probe with an internally linked quencher (exo-IQ). *Clinical Chemistry* 8 May 2020 [Epub ahead of print]:hva116. [DOI: [10.1093/clinchem/hvaa116](https://doi.org/10.1093/clinchem/hvaa116)]

Bordi 2020 {published data only}

Bordi L, Piralla A, Lalle E, Giardina F, Colavita F, Tallarita M, et al. Rapid and sensitive detection of SARS-CoV-2 RNA using the Simplexa COVID-19 direct assay. *Journal of Clinical Virology* 2020;**128**:104416.

Broughton 2020 {published data only}

Broughton JP, Deng X, Yu G, Fasching CL, Singh J, Streithorst J, et al. Rapid detection of 2019 novel coronavirus SARS-CoV-2 using a CRISPR-based DETECTR lateral flow assay. *medRxiv [Preprint]* 27 March 2020:1-28. [DOI: [10.1101/2020.03.06.20032334](https://doi.org/10.1101/2020.03.06.20032334)]

Callahan 2020 {published data only}

Callahan CJ, Lee R, Zulauf K, Tamburello L, Smith KP, Previtera J, et al. Open development and clinical validation of multiple 3D-printed sample-collection swabs: rapid resolution

of a critical COVID-19 testing bottleneck. *medRxiv [Preprint]* 7 May 2020:1-16. [EMBASE: 10.1101/2020.04.14.20065094]

Callahan CJ, Lee R, Zulauf KE, Tamburello L, Smith KP, Previtera J, et al. Open development and clinical validation of multiple 3D-printed nasopharyngeal collection swabs: rapid resolution of a critical COVID-19 testing bottleneck. *Journal of Clinical Microbiology* 2020;**58**(8):e00876-20. [DOI: [10.1128/JCM.00876-20](https://doi.org/10.1128/JCM.00876-20)]

Chandler-Brown 2020 {published data only}

Chandler-Brown D, Bueno AM, Atay O, Tsao DS. A highly scalable and rapidly deployable RNA extraction-free COVID-19 assay by quantitative Sanger sequencing. *medRxiv [Preprint]* 10 April 2020:1-15. [DOI: [10.1101/2020.04.07.029199](https://doi.org/10.1101/2020.04.07.029199)]

Colson 2020 {published data only}

Colson P, Lagier JC, Baudoin JP, Bou Khalil J, La Scola B, Raoult D. Ultrarapid diagnosis, microscope imaging, genome sequencing, and culture isolation of SARS-CoV-2. *European Journal of Clinical Microbiology & Infectious Diseases* 2020;**39**(8):1601-3.

Comar 2020 {published data only}

Comar M, Brumat M, Concas MP, Argentini G, Bianco A, Bicego L, et al. COVID-19 experience: first Italian survey on healthcare staff members from a Mother-Child Research hospital using combined molecular and rapid immunoassays test. *medRxiv [Preprint]* 22 April 2020:1-12. [DOI: [10.1101/2020.04.19.20071563](https://doi.org/10.1101/2020.04.19.20071563)]

Crone 2020 {published data only}

Crone MA, Priestman M, Ciechonska M, Jensen K, Sharp DJ, Randell P, et al. A new role for Biofoundries in rapid prototyping, development, and validation of automated clinical diagnostic tests for SARS-CoV-2. *medRxiv [Preprint]* 12 May 2020:1-31. [DOI: [10.1101/2020.05.02.20088344](https://doi.org/10.1101/2020.05.02.20088344)]

Curti 2020 {published data only}

Curti L, Pereyra-Bonnet F, Gimenez CA. An ultrasensitive, rapid, and portable coronavirus SARS-CoV-2 sequence detection method based on CRISPR-Cas12. *bioRxiv [Preprint]* 2 March 2020:1-10. [DOI: [10.1101/2020.02.29.971127](https://doi.org/10.1101/2020.02.29.971127)]

Ding 2020 {published data only}

Ding X, Yin K, Li Z, Liu C. All-in-One Dual CRISPR-Cas12a (AIOD-CRISPR) assay: a case for rapid, ultrasensitive and visual detection of novel coronavirus SARS-CoV-2 and HIV virus. *bioRxiv [Preprint]* 21 March 2020:1-19. [DOI: [10.1101/2020.03.19.998724](https://doi.org/10.1101/2020.03.19.998724)]

Dohla 2020 {published data only}

Dohla M, Boesecke C, Schulte B, Diegmann C, Sib E, Richter E, et al. Rapid point-of-care testing for SARS-CoV-2 in a community screening setting shows low sensitivity. *Public Health* 2020;**182**:170-2.

Farfan 2020 {published data only}

Farfan MJ, Torres JP, Oryan M, Olivares M, Gallardo P, Salas C. Optimizing RT-PCR detection of SARS-CoV-2 for developing

countries using pool testing. *medRxiv [Preprint]* 17 April 2020:1-10. [DOI: [10.1101/2020.04.15.20067199](https://doi.org/10.1101/2020.04.15.20067199)]

Francis 2020 {published data only}

Francis R, Le Bideau M, Jardot P, Grimaldier C, Raoult D, Khalil JY, et al. High speed large scale automated isolation of SARS-CoV-2 from clinical samples using miniaturized co-culture coupled with high content screening. *bioRxiv [Preprint]* 19 May 2020:1-23. [DOI: [10.1101/2020.05.14.097295](https://doi.org/10.1101/2020.05.14.097295)]

Freire-Paspuel 2020 {published data only}

Freire-Paspuel B, Vega-Marino P, Velez A, Cruz M, Bereguian MA. High sensitivity CDC EUA SARS-CoV-2 kit-based End Point-PCR assay. *medRxiv [Preprint]* 18 May 2020:1-7. [DOI: [10.1101/2020.05.11.20098590](https://doi.org/10.1101/2020.05.11.20098590)]

Ganguli 2020 {published data only}

Ganguli A, Mostafa A, Berger J, Aydin M, Sun F, Valera E, et al. Rapid isothermal amplification and portable detection system for SARS-CoV-2. *bioRxiv [Preprint]* 21 May 2020:1-31. [DOI: [10.1101/2020.05.21.108381](https://doi.org/10.1101/2020.05.21.108381)]

Giamarellos-Bourboulis 2020 {published data only}

Giamarellos-Bourboulis EJ, Netea MG, Rovina N, Akinosoglou K, Antoniadou A, Antonakos N, et al. Complex immune dysregulation in COVID-19 patients with severe respiratory failure. *Cell Host & Microbe* 2020;**27**(6):992-1000 e3.

Gonzalez-Gonzalez 2020 {published data only}

Gonzalez-Gonzalez E, Lara-Mayorga IM, Rodriguez-Sanchez IP, Yee-de Leon F, Garcia-Rubio A, Garciamendez-Mijares CE, et al. Scaling diagnostics in times of COVID-19: rapid prototyping of 3D-printed water circulators for Loop-mediated Isothermal Amplification (LAMP) and detection of SARS-CoV-2 virus. *medRxiv [Preprint]* 19 June 2020:1-39. [DOI: [10.1101/2020.04.09.20058651](https://doi.org/10.1101/2020.04.09.20058651)]

Grant 2020 {published data only}

Grant PR, Turner MA, Shin GY, Nastouli E, Levett LJ. Extraction-free COVID-19 (SARS-CoV-2) diagnosis by RT-PCR to increase capacity for national testing programmes during a pandemic. *bioRxiv [Preprint]* 9 April 2020:1-6.

Hass 2020 {published data only}

Hass KN, Bao M, He Q, Park M, Qin P, Du K. Integrated Micropillar Polydimethylsiloxane Accurate CRISPR Detection (IMPACT) system for rapid viral DNA sensing. *bioRxiv [Preprint]* 20 March 2020:1-10. [DOI: [10.1101/2020.03.17.994137](https://doi.org/10.1101/2020.03.17.994137)]

Hogan 2020a {published data only}

Hogan CA, Sahoo MK, Huang C, Garamani N, Stevens B, Zehnder J, et al. Comparison of the Panther Fusion and a laboratory-developed test targeting the envelope gene for detection of SARS-CoV-2. *Journal of Clinical Virology* 2020;**127**:104383.

Hu 2020 {published data only}

Hu X, Deng Q, Li J, Chen J, Wang Z, Zhang X, et al. Development and clinical application of a rapid and sensitive loop-mediated isothermal amplification test for SARS-CoV-2 infection. *medRxiv [Preprint]* 29 May 2020:1-28. [DOI: [10.1101/2020.05.20.20108530](https://doi.org/10.1101/2020.05.20.20108530)]

Huang 2020 {published data only}

Huang WE, Lim B, Hsu CC, Xiong D, Wu W, Yu Y, et al. RT-LAMP for rapid diagnosis of coronavirus SARS-CoV-2. *Microbial Biotechnology* 2020;**13**(4):950-61.

Jiang 2020 {published data only}

Jiang M, Pan W, Arastehfar A, Fang W, Ling L, Fang H, et al. Development and validation of a rapid single-step reverse transcriptase loop-mediated isothermal amplification (RT-LAMP) system potentially to be used for reliable and high-throughput screening of COVID-19. *medRxiv [Preprint]* 27 March 2020:1-12. [DOI: [10.1101/2020.03.15.20036376](https://doi.org/10.1101/2020.03.15.20036376)]

Joung 2020 {published data only}

Joung J, Ladha A, Saito M, Segel M, Bruneau R, Huang MW, et al. Point-of-care testing for COVID-19 using SHERLOCK diagnostics. *medRxiv [Preprint]* 8 May 2020:1-21. [DOI: [10.1101/2020.05.04.20091231](https://doi.org/10.1101/2020.05.04.20091231)]

Kalikiri 2020 {published data only}

Kalikiri MK, Hasan M, Mirza F, Xaba T, Tang P, Lorenz S. High-throughput extraction of SARS-CoV-2 RNA from nasopharyngeal swabs using solid-phase reverse immobilization beads. *medRxiv [Preprint]* 11 April 2020:1-5. [DOI: [10.1101/2020.04.08.20055731](https://doi.org/10.1101/2020.04.08.20055731)]

Kim 2019 {published data only}

Kim JH, Kang M, Park E, Chung DR, Kim J, Hwang ES. A simple and multiplex Loop-Mediated isothermal Amplification (LAMP) assay for rapid detection of SARS-CoV. *Biochip Journal* 2019;**13**(4):341-51.

Konrad 2020 {published data only}

Konrad R, Eberle U, Dangel A, Treis B, Berger A, Bengs K, et al. Rapid establishment of laboratory diagnostics for the novel coronavirus SARS-CoV-2 in Bavaria, Germany, February 2020. *Euro Surveillance* 2020;**25**(9):2000173.

Kurstjens 2020 {published data only}

Kurstjens S, Van der Horst A, Herpers R, Geerits MW, Kluiters-de Hingh YC, Göttgens E-L, et al. Rapid identification of SARS-CoV-2-infected patients at the emergency department using routine testing. *bioRxiv [Preprint]* 4 April 2020:1-21. [DOI: [10.1101/2020.04.20.20067512](https://doi.org/10.1101/2020.04.20.20067512)]

Lalli 2020 {published data only}

Lalli MA, Chen X, Langmade SJ, Fronick CC, Sawyer CS, Burcea LC, et al. Rapid and extraction-free detection of SARS-CoV-2 from saliva with colorimetric LAMP. *medRxiv [Preprint]* 11 May 2020:1-25. [DOI: [10.1101/2020.05.07.20093542](https://doi.org/10.1101/2020.05.07.20093542)]

Lamb 2020 {published data only}

Lamb LE, Bartolone SN, Ward E, Chancellor MB. Rapid detection of novel coronavirus (COVID-19) by reverse transcription-loop-mediated isothermal amplification. *medRxiv [Preprint]* 24 February 2020:1-17. [DOI: [10.1101/2020.02.19.20025155](https://doi.org/10.1101/2020.02.19.20025155)]

Lee 2020 {published data only}

Lee JY, Best N, McAuley J, Porter JL, Seemann T, Schultz MB, et al. Validation of a single-step, single-tube reverse transcription-loop-mediated isothermal amplification assay for rapid

detection of SARS-CoV-2 RNA. *bioRxiv [Preprint]* 30 April 2020:1-32. [DOI: [10.1101/2020.04.28.067363](https://doi.org/10.1101/2020.04.28.067363)]

Lin 2020 {published data only}

Lin CY, Hwang D, Chiu NC, Weng LC, Liu HF, Mu JJ, et al. Increased detection of viruses in children with respiratory tract infection using PCR. *International Journal of Environmental Research and Public Health* 2020;**17**(2):564.

Lowe 2020 {published data only}

Lowe CF, Matic N, Ritchie G, Lawson T, Stefanovic A, Champagne S, et al. Detection of low levels of SARS-CoV-2 RNA from nasopharyngeal swabs using three commercial molecular assays. *Journal of Clinical Virology* 2020;**128**:104387.

Lu 2020 {published data only}

Lu R, Wu X, Wan Z, Li Y, Zuo L, Qin J, et al. Development of a novel reverse transcription loop-mediated isothermal amplification method for rapid detection of SARS-CoV-2. *Virologica Sinica* 2020;**35**(3):344-7.

Lu 2020a {published data only}

Lu R, Wu X, Wan Z, Li Y, Jin X, Zhang C. A novel reverse transcription loop-mediated isothermal amplification method for rapid detection of SARS-CoV-2. *International Journal of Molecular Sciences* 2020;**21**(8):2826.

Mahari 2020 {published data only}

Mahari S, Roberts A, Shahdeo D, Gandhi S. eCovSens-Ultrasensitive novel in-house built printed circuit board based electrochemical device for rapid detection of nCOVID-19 antigen, a spike protein domain 1 of SARS-CoV-2. *bioRxiv [Preprint]* 11 May 2020:1-20. [DOI: [10.1101/2020.04.24.059204](https://doi.org/10.1101/2020.04.24.059204)]

Marzinotto 2020 {published data only}

Marzinotto S, Mio C, Cifu A, Verardo R, Pipan C, Schneider C, et al. A streamlined approach to rapidly detect SARS-CoV-2 infection, avoiding RNA extraction. *medRxiv [Preprint]* 11 April 2020:1-10. [DOI: [10.1101/2020.04.06.20054114](https://doi.org/10.1101/2020.04.06.20054114)]

McCormick-Baw 2020 {published data only}

McCormick-Baw C, Morgan K, Gaffney D, Cazares Y, Jaworski K, Byrd A, et al. Saliva as an alternate specimen source for detection of SARS-CoV-2 in symptomatic patients using Cepheid Xpert Xpress SARS-CoV-2. *Journal of Clinical Microbiology* 2020;**58**(8):e01109-20. [DOI: [10.1128/JCM.01109-20](https://doi.org/10.1128/JCM.01109-20)]

McRae 2020 {published data only}

McRae MP, Simmons GW, Christodoulides NJ, Lu Z, Kang SK, Fenyo D, et al. Clinical decision support tool and rapid point-of-care platform for determining disease severity in patients with COVID-19. *medRxiv [Preprint]* 22 April 2020:1-32. [DOI: [10.1101/2020.04.16.20068411](https://doi.org/10.1101/2020.04.16.20068411)]

Mei 2020 {published data only}

Mei X, Lee HC, Diao K, Huang M, Lin B, Liu C, et al. Artificial intelligence-enabled rapid diagnosis of COVID-19 patients. *medRxiv [Preprint]* 7 May 2020:1-30. [DOI: [10.1101/2020.04.12.20062661](https://doi.org/10.1101/2020.04.12.20062661)]

Noerz 2020 {published data only}

Noerz D, Fischer N, Schultze A, Kluge S, Mayer-Runge U, Aepfelbacher M, et al. Clinical evaluation of a SARS-CoV-2 RT-PCR assay on a fully automated system for rapid on-demand testing in the hospital setting. *Journal of Clinical Virology* 2020;**128**:104390.

Osterdahl 2020 {published data only}

Osterdahl MF, Lee KA, Ni LM, Wilson S, Douthwaite S, Horsfall R, et al. Detecting SARS-CoV-2 at point of care: preliminary data comparing Loop-mediated Isothermal Amplification (LAMP) to PCR. *medRxiv [Preprint]* 4 April 2020:1-9. [DOI: [10.1101/2020.04.01.20047357](https://doi.org/10.1101/2020.04.01.20047357)]

Paden 2020 {published data only}

Paden CR, Tao Y, Queen K, Zhang J, Li Y, Uehara A, et al. Rapid, sensitive, full genome sequencing of severe acute respiratory syndrome virus coronavirus 2 (SARS-CoV-2). *bioRxiv [Preprint]* 24 April 2020:1-13. [DOI: [10.1101/2020.04.22.055897](https://doi.org/10.1101/2020.04.22.055897)]

Pellanda 2020 {published data only}

Pellanda LC, Wendland EM, McBride AJ, Tovo-Rodrigues L, Ferreira MR, Dellagostin OA, et al. Sensitivity and specificity of a rapid test for assessment of exposure to SARS-CoV-2 in a community-based setting in Brazil. *medRxiv [Preprint]* 10 May 2020:1-10. [DOI: [10.1101/2020.05.06.20093476](https://doi.org/10.1101/2020.05.06.20093476)]

Pfefferle 2020 {published data only}

Pfefferle S, Reucher S, Norz D, Lutgehetmann M. Evaluation of a quantitative RT-PCR assay for the detection of the emerging coronavirus SARS-CoV-2 using a high throughput system. *EuroSurveillance* 2020;**25**(9):2000152.

Seo 2020 {published data only}

Seo G, Lee G, Kim MJ, Baek SH, Choi M, Ku KB, et al. Rapid detection of COVID-19 causative virus (SARS-CoV-2) in human nasopharyngeal swab specimens using field-effect transistor-based biosensor. *ACS Nano* 2020;**14**(4):5135-42.

Smyrlaki 2020 {published data only}

Smyrlaki I, Ekman M, Lentini A, Vondracek M, Papanicolaou N, Aarum J, et al. Massive and rapid COVID-19 testing is feasible by extraction-free SARS-CoV-2 RT-qPCR. *medRxiv [Preprint]* 12 May 2020:1-18. [DOI: [10.1101/2020.04.17.20067348](https://doi.org/10.1101/2020.04.17.20067348)]

St Hilaire 2020 {published data only}

St Hilaire BG, Durand NC, Mitra N, Pulido SG, Mahajan R, Blackburn A, et al. A rapid, low cost, and highly sensitive SARS-CoV-2 diagnostic based on whole genome sequencing. *bioRxiv [Preprint]* 11 May 2020:1-29. [DOI: [10.1101/2020.04.25.061499](https://doi.org/10.1101/2020.04.25.061499)]

Tan 2020 {published data only}

Tan X, Lin C, Zhang J, Khaing OM, Fan X. Rapid and quantitative detection of COVID-19 markers in micro-liter sized samples. *bioRxiv [Preprint]* 22 April 2020:1-17. [DOI: [10.1101/2020.04.20.052233](https://doi.org/10.1101/2020.04.20.052233)]

Visseaux 2020 {published data only}

Visseaux B, Le Hingrat Q, Collin G, Bouzid D, Lebourgeois S, Le Pluart D, et al. Evaluation of the QIAstat-Dx Respiratory SARS-CoV-2 Panel, the first rapid multiplex PCR commercial

assay for SARS-CoV-2 detection. *Journal of Clinical Microbiology* 2020;**58**(8):e00630-20. [DOI: [10.1128/JCM.00630-20](https://doi.org/10.1128/JCM.00630-20)]

Wang 2020 {published data only}

Wang X, Zhong M, Liu Y, Ma P, Dang L, Meng Q, et al. Rapid and sensitive detection of COVID-19 using CRISPR/Cas12a-based detection with Naked Eye Readout, CRISPR/Cas12a-NER. *Science Bulletin (Beijing)* 5 May 2020 [Epub ahead of print]. [DOI: [10.1016/j.scib.2020.04.041](https://doi.org/10.1016/j.scib.2020.04.041)]

Wang 2020a {published data only}

Wang X, Yao H, Xu X, Zhang P, Zhang M, Shao J, et al. Limits of detection of six approved RT-PCR kits for the novel SARS-coronavirus-2 (SARS-CoV-2). *Clinical Chemistry* 2020;**66**(7):977-9. [DOI: [10.1093/clinchem/hvaa099](https://doi.org/10.1093/clinchem/hvaa099)]

Wee 2020 {published data only}

Wee SK, Sivalingam SP, Yap EPH. Rapid direct nucleic acid amplification test without RNA extraction for SARS-CoV-2 using a portable PCR thermocycler. *bioRxiv [Preprint]* 20 April 2020:1-12. [DOI: [10.1101/2020.04.17.042366](https://doi.org/10.1101/2020.04.17.042366)]

Xue 2020 {published data only}

Xue G, Li S, Zhang W, Du B, Cui J, Yan C, et al. Reverse-transcription recombinase-aided amplification assay for rapid detection of the 2019 novel coronavirus (SARS-CoV-2). *Analytical Chemistry* 2020;**92**(14):9699-705. [DOI: [10.1021/acs.analchem.0c01032](https://doi.org/10.1021/acs.analchem.0c01032)]

Yan 2020 {published data only}

Yan C, Cui J, Huang L, Du B, Chen L, Xue G, et al. Rapid and visual detection of 2019 novel coronavirus (SARS-CoV-2) by a reverse transcription loop-mediated isothermal amplification assay. *Clinical Microbiology and Infection* 2020;**26**(6):773-9.

Yang 2020 {published data only}

Yang W, Dang X, Wang Q, Xu M, Zhao Q, Zhou Y, et al. Rapid detection of SARS-CoV-2 using reverse transcription RT-LAMP method. *medRxiv [Preprint]* 3 March 2020:1-25. [DOI: [10.1101/2020.03.02.20030130](https://doi.org/10.1101/2020.03.02.20030130)]

Yu 2020 {published data only}

Yu L, Wu S, Hao X, Dong X, Mao L, Pelechano V, et al. Rapid detection of COVID-19 coronavirus using a Reverse Transcriptional Loop-Mediated Isothermal Amplification (RT-LAMP) diagnostic platform. *Clinical Chemistry* 2020;**66**(7):975-7.

Yu 2020a {published data only}

Yu L, Wu S, Hao X, Li X, Liu X, Ye S, et al. Rapid colorimetric detection of COVID-19 coronavirus using a Reverse Transcriptional Loop-Mediated Isothermal Amplification (RT-LAMP) diagnostic platform: iLACO. *medRxiv [Preprint]* 24 February 2020:1-19. [DOI: [10.1101/2020.02.20.20025874](https://doi.org/10.1101/2020.02.20.20025874)]

Zamecnik 2020 {published data only}

Zamecnik CR, Rajan JV, Yamauchi KA, Mann SA, Sowa GM, Zorn KC, et al. ReScan, a multiplex diagnostic pipeline, pans human sera for SARS-CoV-2 antigens. *medRxiv [Preprint]* 13 May 2020:1-21. [DOI: [10.1101/2020.05.11.20092528](https://doi.org/10.1101/2020.05.11.20092528)]

Zeng 2020 {published data only}

Zeng W, Liu G, Ma H, Zhao D, Yang Y, Liu M, et al. Biochemical characterization of SARS-CoV-2 nucleocapsid protein. *Biochemical and Biophysical Research Communications* 2020;**527**(3):618-23.

Zhang 2020 {published data only}

Zhang Y, Odiwuor N, Xiong J, Sun L, Nyaruaba RO, Wei H, et al. Rapid molecular detection of SARS-CoV-2 (COVID-19) virus RNA using colorimetric LAMP. *medRxiv [Preprint]* 29 February 2020:1-14. [DOI: [10.1101/2020.02.26.20028373](https://doi.org/10.1101/2020.02.26.20028373)]

Zhao 2020 {published data only}

Zhao Z, Cui H, Song W, Ru X, Zhou W, Yu X. A simple magnetic nanoparticles-based viral RNA extraction method for efficient detection of SARS-CoV-2. *bioRxiv [Preprint]* 27 February 2020:1-18. [DOI: [10.1101/2020.02.22.961268](https://doi.org/10.1101/2020.02.22.961268)]

Additional references

Arevalo-Rodriguez 2020

Arevalo-Rodriguez I, Buitrago-Garcia D, Simancas-Racines D, Zambrano-Achig P, del Campo R, Ciapponi A, et al. False-negative results of initial RT-PCR assays for COVID-19: a systematic review. *medRxiv [Preprint]* 2020:1-26. [DOI: [10.1101/2020.04.16.20066787](https://doi.org/10.1101/2020.04.16.20066787)]

Bossuyt 2015

Bossuyt PM, Reitsma JB, Bruns DE, Gatsonis CA, Glasziou PP, Irwig L, et al. STARD 2015: an updated list of essential items for reporting diagnostic accuracy studies. *BMJ* 2015;**351**:h5527. [DOI: [10.1136/bmj.h5527](https://doi.org/10.1136/bmj.h5527)] [PMID: 26511519]

Carter 2020

Carter LJ, Garner LV, Smoot JW, Li Y, Zhou Q, Saveson CJ, et al. Assay techniques and test development for COVID-19 diagnosis. *ACS Central Science* 2020;**6**(5):591-605. [DOI: [10.1021/acscentsci.0c00501](https://doi.org/10.1021/acscentsci.0c00501)]

Cheng 2020

Cheng MP, Yansouni CP, Basta NE, Desjardins M, Kanjilal S, Paquette K, et al. Serodiagnostics for severe acute respiratory syndrome-related coronavirus-2: a narrative review. *Annals of Internal Medicine* (in press).

Corman 2020

Corman V, Bleicker T, Brünink S, Drosten C, Landt O, Koopmans M, et al. Diagnostic detection of Wuhan coronavirus 2019 by real-time RT-PCR - protocol and preliminary evaluation as of Jan 13, 2020. Available from www.who.int/docs/default-source/coronaviruse/wuhan-virus-assay-v1991527e5122341d99287a1b17c111902.pdf?sfvrsn=d381fc88_2 2020.

Covidence [Computer program]

Veritas Health Innovation Covidence. Version accessed 27 April 2020. Melbourne, Australia: Veritas Health Innovation. Available at covidence.org.

Deeks 2020

Deeks JJ, Dinnes J, Takwoingi Y, Davenport C, Leeftang MM, Spijker R, et al. Diagnosis of SARS-CoV-2 infection and COVID-19: accuracy of signs and symptoms; molecular, antigen, and antibody tests; and routine laboratory markers. *Cochrane Database of Systematic Reviews* 2020, Issue 4. Art. No: CD013596. [DOI: [10.1002/14651858.CD013596](https://doi.org/10.1002/14651858.CD013596)]

Deeks 2020a

Deeks JJ, Dinnes J, Takwoingi Y, Davenport C, Spijker R, Taylor-Phillips S, et al. Antibody tests for identification of current and past infection with SARS-CoV-2. *Cochrane Database of Systematic Reviews* 2020, Issue 6. Art. No: CD013652. [DOI: [10.1002/14651858.CD013652](https://doi.org/10.1002/14651858.CD013652)]

FIND 2020

FIND. SARS-COV-2 Diagnostic pipeline. www.finddx.org/covid-19/pipeline/ Accessed 19 July 2020.

Green 2020

Green K, Graziadio S, Turner P, Fanshawe T, Allen J, on behalf of the Oxford COVID-19 Evidence Service Team Centre. Molecular and antibody point-of-care tests to support the screening, diagnosis and monitoring of COVID-19. Available at www.cebm.net/oxford-covid-19/ 7 April 2020.

Hadgu 1999

Hadgu A. Discrepant analysis: a biased and an unscientific method for estimating test sensitivity and specificity. *Journal of Clinical Epidemiology* 1999;**52**(12):1231-7. [DOI: [10.1016/S0895-4356\(99\)00101-8](https://doi.org/10.1016/S0895-4356(99)00101-8)]

Kozel 2017

Kozel TR, Burnham-Marusch AR. Point-of-care testing for infectious diseases: past, present, and future. *Journal of Clinical Microbiology* 2017;**55**(8):2313-20. [DOI: [10.1128/JCM.00476-17](https://doi.org/10.1128/JCM.00476-17)]

Leeftang 2013

Leeftang MM, Rutjes AW, Reitsma JB, Hooft L, Bossuyt PM. Variation of a test's sensitivity and specificity with disease prevalence. *CMAJ : Canadian Medical Association Journal* 2013;**185**(11):E537-44. [PMID: 23798453]

McInnes 2018

McInnes MD, Moher D, Thombs BD, McGrath TA, Bossuyt PM, PRISMA-DTA Group. Preferred reporting items for a systematic review and meta-analysis of diagnostic test accuracy studies: the PRISMA-DTA Statement. *JAMA* 2018;**319**(4):388-96. [DOI: [10.1001/jama.2017.19163](https://doi.org/10.1001/jama.2017.19163)] [PMID: 29362800]

McInnes 2020

McInnes M, Leeftang MM, Salameh J-P, McGrath T, Van der Pol CB, Frank RA, et al. Imaging tests for the diagnosis of COVID-19. *Cochrane Database of Systematic Reviews* 2020, Issue 6. Art. No: CD013639. [DOI: [10.1002/14651858.CD013639](https://doi.org/10.1002/14651858.CD013639)]

Moher 2009

Moher D, Liberati A, Tetzlaff J, Altman DG, The PRISMA Group. Preferred reporting items for systematic reviews and meta-analyses: the PRISMA Statement. *PLoS Medicine* 2009;**6**(7):1000097. [DOI: [10.1371/journal.pmed1000097](https://doi.org/10.1371/journal.pmed1000097)]

Pai 2012

Pai NP, Vadnais C, Denkinger C, Engel N, Pai M. Point-of-care testing for infectious diseases: diversity, complexity, and barriers in low- and middle-income countries. *PLoS Medicine* 2012;**9**(9):e1001306.

Reitsma 2005

Reitsma JB, Glas AS, Rutjes AW, Scholten RJ, Bossuyt PM, Zwinderman AH. Bivariate analysis of sensitivity and specificity produces informative summary measures in diagnostic reviews. *Journal of Clinical Epidemiology* 2005;**58**(10):982-90. [DOI: [10.1016/j.jclinepi.2005.02.022](https://doi.org/10.1016/j.jclinepi.2005.02.022)]

Review Manager 2014 [Computer program]

Nordic Cochrane Centre, The Cochrane Collaboration Review Manager 5 (RevMan 5). Version 5.3. Copenhagen: Nordic Cochrane Centre, The Cochrane Collaboration, 2014.

Stata [Computer program]

Stata. Version 15. College Station, TX, USA: StataCorp, 2017. Available at www.stata.com.

Struyf 2020

Struyf T, Deeks JJ, Dinnes J, Takwoingi Y, Davenport C, Leeflang MM, et al. Signs and symptoms to determine if a patient presenting in primary care or hospital outpatient settings has COVID-19 disease. *Cochrane Database of Systematic Reviews* 2020, Issue 7. Art. No: CD013665. [DOI: [10.1002/14651858.CD013665](https://doi.org/10.1002/14651858.CD013665)]

Subsoontorn 2020

Subsoontorn P, Lohitnavy M, Kongkaew C. The diagnostic accuracy of nucleic acid point-of-care tests for human coronavirus: a systematic review and meta-analysis. *medRxiv [Preprint]* 2020. [DOI: [10.1101/2020.07.09.20150235](https://doi.org/10.1101/2020.07.09.20150235)]

Takwoingi 2017

Takwoingi Y, Guo B, Riley RD, Deeks JJ. Performance of methods for meta-analysis of diagnostic test accuracy with few studies or sparse data. *Statistical Methods in Medical Research* 2017;**26**(4):1896-911.

Usher-Smith 2016

Usher-Smith JA, Sharp SJ, Griffin SJ. The spectrum effect in tests for risk prediction, screening, and diagnosis. *BMJ* 2016;**353**:i3139. [DOI: [10.1136/bmj.i3139](https://doi.org/10.1136/bmj.i3139)]

Whiting 2011

Whiting PF, Rutjes AW, Westwood ME, Mallett S, Deeks JJ, Reitsma JB, et al. QUADAS-2: a revised tool for the quality assessment of diagnostic accuracy studies. *Annals of Internal Medicine* 2011;**155**(8):529-36.

WHO 2018

World Health Organization (WHO). Diagnostic assessment: in vitro diagnostic medical devices (IVDs) used for the detection of high-risk human papillomavirus (HPV) genotypes in cervical cancer screening. Licence: CC BY-NC-SA 3.0 IGO. Available at apps.who.int/iris/handle/10665/272282 2018.

WHO 2020a

World Health Organization. Laboratory testing of 2019 novel coronavirus (2019-nCoV) in suspected human cases: interim guidance. Available from www.who.int/publications/i/item/laboratory-testing-for-2019-novel-coronavirus-in-suspected-human-cases-20200117 2020.

WHO 2020b

Global surveillance for COVID-19 caused by human infection with COVID-19 virus: interim guidance. Available from www.who.int/publications/i/item/global-surveillance-for-covid-19-caused-by-human-infection-with-covid-19-virus-interim-guidance 2020.

WHO 2020c

COVID-19 Target product profiles for priority diagnostics to support response to the COVID-19 pandemic v.0.1. Available from www.who.int/publications/m/item/covid-19-target-product-profiles-for-priority-diagnostics-to-support-response-to-the-covid-19-pandemic-v-0-1 2020.

Zheng 2020

Zheng S, Fan J, Yu F, Feng B, Lou B, Zou Q, et al. Viral load dynamics and disease severity in patients infected with SARS-CoV-2 in Zhejiang province, China, January-March 2020: retrospective cohort study. *BMJ* 2020;**369**:m1443.

* Indicates the major publication for the study

CHARACTERISTICS OF STUDIES

Characteristics of included studies [ordered by study ID]

Assennato 2020

Study characteristics

Patient Sampling

Single-group study to estimate sensitivity and specificity:
- samples from symptomatic individuals with suspected COVID-19 sent for routine laboratory diagnosis; supplied via PHE (n = 172)

Recruitment: not stated

Assennato 2020 (Continued)

	<p>Prospective or retrospective: retrospective</p> <p>Number of samples (samples with confirmed SARS-CoV-2): 172 (88)</p>
Patient characteristics and setting	<p>Setting: not stated; supplied by PHE</p> <p>Location: PHE, Cambridge Laboratory (samples from East of England)</p> <p>Country: UK</p> <p>Dates: not stated</p> <p>Symptoms and severity: symptomatic; no further details</p> <p>Demographics: not stated</p> <p>Exposure history: not stated</p>
Index tests	<p>Test name: SAMBA II SARS-CoV-2 Test</p> <p>Manufacturer: Diagnostics for the Real World</p> <p>Antigen target: ORF1ab, N2</p> <p>Antibody: N/A</p> <p>Test method: rapid PCR</p> <p>Samples used: combined nose and throat swab samples, provided as VTM</p> <p>Transport media: samples diluted 1:2 with SAMBA SCoV buffer</p> <p>Sample storage: not stated</p> <p>Test operator: not stated; presume laboratory staff</p> <p>Definition of test positivity: as per manufacturer; either target present</p> <p>Blinding reported: yes; states that samples were rendered anonymous and provided blinded for the purpose of test validation</p> <p>Timing of samples: not stated</p>
Target condition and reference standard(s)	<p>Reference standard: RT-PCR; (1) Cambridge RdRp gene (Wuhan) assay on the Rotor gene Q real-time PCR assay routinely used by PHE; Ct ≤ 36 considered positive. (2) Samples also tested with the PHE Colindale (Reference Laboratory) assay</p> <p>Definition of non-COVID cases: Single RT-PCR negative</p> <p>Genetic target(s): (1) RdRp, E gene, (2) RdRp 'different region'</p> <p>Samples used: combined nose and throat swab in VTM; same as for index test</p> <p>Timing of reference standard: not stated; Cambridge assay seems to have been part of routine testing near to time of sample collection; not clear if Colindale assay was at a later date after a period of storage</p> <p>Blinded to index test: not stated but seems yes for Cambridge assay</p> <p>Incorporated index test: no</p>
Flow and timing	<p>Time interval between index and reference tests: not stated; seems likely reference was carried out for routine diagnostic testing</p> <p>All participants received same reference standard: yes (all samples underwent both RT-PCR tests)</p>

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Assennato 2020 (Continued)

Missing data: none reported

Uninterpretable results: none reported

Indeterminate results (index test): 3 FP and 1 FN result retested using SAMBA-II; same results obtained on repeat

Indeterminate results (reference standard): 3 FP and 1 FN result were re-tested
- all 3 FPS found to be borderline positive for ≥ 1 target gene on either Colindale or Cambridge (Wuhan) test (reclassified as TP)
- the FN result remained positive on both RT-PCR assays

Unit of analysis: refers to participants rather than samples

Comparative

Notes

Funding: RKG is funded by Wellcome Senior Fellowship In Clinical Science award no WT108082AIA

Publication status: preprint

Source: medRxiv

Author COI: no COI statement reported; 3 co-authors are affiliated to test manufacturer

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	Yes		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		Unclear risk	
Are there concerns that the included patients and setting do not match the review question?			Unclear
DOMAIN 2: Index Test (Antigen tests)			
DOMAIN 2: Index Test (Rapid PCR tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Yes		
If a threshold was used, was it pre-specified?	Yes		

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Assennato 2020 (Continued)

Could the conduct or interpretation of the index test have introduced bias?		Low risk
Are there concerns that the index test, its conduct, or interpretation differ from the review question?		Unclear
DOMAIN 3: Reference Standard		
Is the reference standards likely to correctly classify the target condition?	No	
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes	
Reference standard does not incorporate result of index test?	Yes	
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk
Are there concerns that the target condition as defined by the reference standard does not match the question?		High
DOMAIN 4: Flow and Timing		
Was there an appropriate interval between index test and reference standard?	Yes	
Did all patients receive the same reference standard?	Yes	
Were all patients included in the analysis?	Unclear	
Did all participants receive a reference standard?	Yes	
Were results presented per patient?	Yes	
Could the patient flow have introduced bias?		Unclear risk

Broder 2020

Study characteristics

Patient Sampling	<p>Single-group study to estimate sensitivity: - samples positive on Roche cobas 6800 assay in lower range of viral load (E target Ct \geq 30) (n = 35)</p> <p>Recruitment: not stated; deliberate sampling according to viral load</p> <p>Prospective or retrospective: unclear</p>
------------------	---

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Broder 2020 (Continued)

	Number of samples (samples with confirmed SARS-CoV-2): 35 (35)
Patient characteristics and setting	<p>Setting: not stated</p> <p>Location: not stated; author institution Emory University School of Medicine, Atlanta</p> <p>Country: USA</p> <p>Dates: not stated</p> <p>Symptoms and severity: not stated; lower viral load</p> <p>Demographics: not stated</p> <p>Exposure history: not stated</p>
Index tests	<p>Test name: GeneXpert Xpress SARS-CoV-2 assay (no product code reported)</p> <p>Manufacturer: Cepheid</p> <p>Antigen target: not stated E gene</p> <p>Antibody: N/A</p> <p>Test method: rapid PCR</p> <p>Samples used: NP swabs in VTM</p> <p>Transport media: not stated</p> <p>Sample storage: within 3 days of initial testing (with RT-PCR)</p> <p>Test operator: not stated; presume laboratory staff</p> <p>Definition of test positivity: not stated; "all specimens were tested using the manufacturer's protocol", no mention of presumptive positives</p> <p>Blinding reported: not stated</p> <p>Timing of samples: not stated</p>
Target condition and reference standard(s)	<p>Reference standard: Roche cobas 6800 SARS-CoV-2 assay</p> <p>Definition of non-COVID cases: N/A</p> <p>Genetic target(s): E gene (unclear if other genetic targets as well)</p> <p>Samples used: NP swabs (as for index test)</p> <p>Timing of reference standard: not stated; presume on presentation</p> <p>Blinded to index test: not stated; presume yes</p> <p>Incorporated index test: no</p>
Flow and timing	<p>Time interval between index and reference tests: same samples; index within 3 days of reference</p> <p>All participants received same reference standard: yes</p> <p>Missing data: none reported</p> <p>Uninterpretable results: none reported</p> <p>Indeterminate results (index test): none reported</p>

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Broder 2020 (Continued)

Indeterminate results (reference standard): discrepancies resolved using modified CDC RT-PCR; 1 FN confirmed as disease negative (i.e. a TN)

Unit of analysis: not stated; refers only to samples

Comparative

Notes

Funding: no funding described

Publication status: accepted manuscript

Source: Journal of Clinical Microbiology

Author COI: Dr. Kraft participated on a Roche advisory board regarding COVID serology. All other study authors have no conflicts

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	No		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (Antigen tests)			
DOMAIN 2: Index Test (Rapid PCR tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Unclear
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		

Broder 2020 (Continued)

Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear
Reference standard does not incorporate result of index test?	Yes
Could the reference standard, its conduct, or its interpretation have introduced bias?	Unclear risk
Are there concerns that the target condition as defined by the reference standard does not match the question?	High
DOMAIN 4: Flow and Timing	
Was there an appropriate interval between index test and reference standard?	Yes
Did all patients receive the same reference standard?	Yes
Were all patients included in the analysis?	Unclear
Did all participants receive a reference standard?	Yes
Were results presented per patient?	Unclear
Could the patient flow have introduced bias?	Unclear risk

Diao 2020

Study characteristics

Patient Sampling	<p>Single group estimating sensitivity and specificity for detecting active disease - samples from cases of suspected SARS-CoV-2 infection (n = 239)</p> <p>Recruitment: not stated if participants were consecutive</p> <p>Prospective or retrospective: retrospective</p> <p>Number of samples (samples with confirmed SARS-CoV-2): 239 (208)</p>
Patient characteristics and setting	<p>Setting: hospital (inpatients)</p> <p>Location: 7 centres, including General Hospital of Central Theatre Command, Wuhan No.7 People's Hospital, Wuhan Pulmonary Hospital, Hubei Maternal and Child Hospital, Taikang Hospital, Hanyang Hospital and Wuguo Hospital. Urine study done in Southwest Hospital in Chongqing</p> <p>Country: China</p> <p>Dates: not stated</p> <p>Symptoms and severity: not stated</p> <p>Demographics: not stated</p>

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Diao 2020 (Continued)

	Exposure history: not stated
Index tests	<p>Test name: not stated</p> <p>Manufacturer: in house (but study authors affiliated to Bioeasy Technology)</p> <p>Antibody: monoclonal antibody</p> <p>Antigen target: nucleocapsid protein (N-antigen)</p> <p>Test method: FIA (fluorescence immunochromatographic); requires immunofluorescence analyser</p> <p>Samples used: NP (all), urine (subgroup)</p> <p>Transport media: samples diluted and mixed in 500 µL saline solution; 100 µL transferred to the sample well of the test card</p> <p>Sample storage: not reported</p> <p>Test operator: not stated; presume laboratory staff</p> <p>Definition of test positivity: cut-off value was determined by testing 100 nasal swab samples of healthy people and calculated as the mean value of the fluorescence signal plus 5 SD.</p> <p>Blinding reported: done in parallel; blinded</p> <p>Timing of samples: not stated</p>
Target condition and reference standard(s)	<p>Reference standard: RT-PCR (Daan Gene kit); performed on ABI Prism 7500 and Light Cycler 480 real-time PCR system. Threshold < 40 Ct; threshold < 30 Ct also investigated</p> <p>Definition of non-COVID cases: all participants underwent 3 nucleic acid tests, and the results of each nucleic acid test were verified by 2 COVID-19 nucleic acid test kits.</p> <p>Genetic target(s): ORF1ab and N gene</p> <p>Samples used: NP swab, same as for index test</p> <p>Timing of reference standard: not stated</p> <p>Blinded to index test: done in parallel; blinded</p> <p>Incorporated index test: no</p>
Flow and timing	<p>Time interval between index and reference tests: done in parallel</p> <p>All participants received same reference standard: yes</p> <p>Missing data: not reported</p> <p>Uninterpretable results: not reported</p> <p>Indeterminate results (index test): none reported</p> <p>Indeterminate results (reference standard): none described</p> <p>Unit of analysis: participants</p>
Comparative	
Notes	<p>Funding: this research was supported by grants from National Key R&D Program of China (2016YFA0502204); Chongqing Health Commission COVID-19 Project (2020ZX01).</p>

Diao 2020 (Continued)

Publication status: preprint (not peer-reviewed)

Source: medRxiv preprint

Author COI: study authors declare no COI present; 1 affiliated to Shenzhen Bioeasy Biotechnology Co. Ltd.

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	Yes		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		Unclear risk	
Are there concerns that the included patients and setting do not match the review question?			Unclear
DOMAIN 2: Index Test (Antigen tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 2: Index Test (Rapid PCR tests)			
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		

Diao 2020 (Continued)

Reference standard does not incorporate re-
sult of index test? Yes

**Could the reference standard, its conduct,
or its interpretation have introduced
bias?**

Low risk

**Are there concerns that the target condi-
tion as defined by the reference standard
does not match the question?**

High

DOMAIN 4: Flow and Timing

Was there an appropriate interval between
index test and reference standard? Yes

Did all patients receive the same reference
standard? Yes

Were all patients included in the analysis? Unclear

Did all participants receive a reference stan-
dard? Yes

Were results presented per patient? Yes

**Could the patient flow have introduced
bias?**

Unclear risk

Harrington 2020

Study characteristics

Patient Sampling

Single-group study to estimate sensitivity and specificity:
- symptomatic patients meeting diagnostic criteria for COVID-19 (n = 524)

Recruitment: consecutive

Prospective or retrospective: unclear; presume prospective

Number of samples (samples with confirmed SARS-CoV-2): 524 (186)

Patient characteristics and setting

Setting: ED (n = 3) or urgent (immediate) care centres (n = 2)

Location: not stated; author institutions Loyola University Medical Centre, Cedars-Si-
nai Medical Centre

Country: USA

Dates: not reported

Symptoms and severity: not stated

Demographics: not stated

Exposure history: not stated

Index tests

Test name: ID NOW COVID-19 assay (no product code provided)

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Harrington 2020 (Continued)

	<p>Manufacturer: Abbott</p> <p>Antigen target: not stated</p> <p>Antibody: N/A</p> <p>Test method: not stated; isothermal PCR</p> <p>Samples used: nasal swabs (provider collected)</p> <p>Transport media: none; direct testing after heat inactivation</p> <p>Sample storage: ED swabs transported in sterile transport containers (using cups or conical tubes)</p> <p>Test operator: on-site medical personnel (urgent care centres); laboratory personnel at each separate location (EDs)</p> <p>- 2 sites reportedly experienced users of ID NOW (one ED and one urgent care centre) and 3 sites received training)</p> <p>Definition of test positivity: as per manufacturer</p> <p>Blinding reported: yes (RT-PCR performed at separate central lab)</p> <p>Timing of samples: not stated; on presentation</p>
Target condition and reference standard(s)	<p>Reference standard: RT-PCR (Abbott RealTime SARS-CoV-2 (ACOV) assay performed on the Abbott m2000 system (Abbott Molecular Inc. Des Plaines, IL); threshold not stated</p> <p>Definition of non-COVID cases: not specifically stated; presume yes as central lab used</p> <p>Genetic target(s): not stated</p> <p>Samples used: NP swabs</p> <p>Timing of reference standard: VTM (no detail)</p> <p>Blinded to index test: not stated, transferred to central clinical laboratory; samples heat inactivated for 30 min at 60 °C prior to testing</p> <p>Incorporated index test: no (paired collection with swabs for index test)</p>
Flow and timing	<p>Time interval between index and reference tests: simultaneous swab collection (different swabs for index and reference)</p> <p>All participants received same reference standard: yes</p> <p>Missing data: none reported</p> <p>Uninterpretable results: none reported</p> <p>Indeterminate results (index test): none reported</p> <p>Indeterminate results (reference standard): 2 initial FPs had repeat sampling:</p> <ul style="list-style-type: none"> - 1 retested on RT-PCR only and was positive (designated as TP) - 1 retested on RT-PCR and ID NOW and was negative on both (designated as FP based on original sampling) <p>Unit of analysis: participants</p>
Comparative	
Notes	<p>Funding: study authors received "received no specific grant from any funding agency in the public, commercial, or not-for-profit sectors"</p>

Harrington 2020 (Continued)

Publication status: accepted manuscript

Source: Journal of Clinical Microbiology

Author COI: COI not mentioned

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Yes		
Was a case-control design avoided?	Yes		
Did the study avoid inappropriate exclusions?	Yes		
Did the study avoid inappropriate inclusions?	Yes		
Could the selection of patients have introduced bias?		Low risk	
Are there concerns that the included patients and setting do not match the review question?			Low concern
DOMAIN 2: Index Test (Antigen tests)			
DOMAIN 2: Index Test (Rapid PCR tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Yes		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Low risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		

Harrington 2020 (Continued)

Reference standard does not incorporate result of index test? Yes

Could the reference standard, its conduct, or its interpretation have introduced bias? High risk

Are there concerns that the target condition as defined by the reference standard does not match the question? High

DOMAIN 4: Flow and Timing

Was there an appropriate interval between index test and reference standard? Yes

Did all patients receive the same reference standard? Yes

Were all patients included in the analysis? Yes

Did all participants receive a reference standard? Yes

Were results presented per patient? Yes

Could the patient flow have introduced bias? Low risk

Hogan 2020
Study characteristics

Patient Sampling	<p>Single-group design to estimate sensitivity and specificity - samples from adult patients from 1 hospital and paediatric and adult samples from surrounding hospitals</p> <p>Recruitment: unclear; equal numbers of positive and negative RT-PCR samples (suspect deliberate sampling by PCR result)</p> <p>Prospective or retrospective: not stated</p> <p>Number of samples (samples with confirmed SARS-CoV-2): 100 (50)</p>
Patient characteristics and setting	<p>Setting: hospital; not stated if inpatient or outpatient (samples selected from clinical virology laboratory)</p> <p>Location: Stanford Health Care (hospital), and surrounding hospitals (not named)</p> <p>Country: USA</p> <p>Dates: 7-13 April 2020</p> <p>Symptoms and severity: not stated</p> <p>Demographics: not stated</p> <p>Exposure history: not stated</p>

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Hogan 2020 (Continued)

Index tests	<p>Test name: Accula SARS-CoV-2 POCT (no product code reported)</p> <p>Manufacturer: Mesa Biotech, Inc., San Diego, CA</p> <p>Antigen target: N gene</p> <p>Antibody: N/A</p> <p>Test method: rapid PCR</p> <p>Samples used: NP swabs in VTM (n = 37) or saline (n = 63, including 37 positive on RT-PCR)</p> <p>Transport media: not stated; 10 µL of VTM or saline was transferred to 60 µL of SARS-CoV-2 buffer within a biosafety cabinet (not covered by manufacturer IFU)</p> <p>Sample storage: not stated; testing appears to have been conducted soon after sample collection</p> <p>Test operator: not stated; presume laboratory staff</p> <p>Definition of test positivity: as per manufacturer</p> <p>Blinding reported: not stated</p> <p>Timing of samples: not stated</p>
Target condition and reference standard(s)	<p>Reference standard: RT-PCR; in-house SHC assay (cites Hogan 2020 10.1016/j.jcv.2020.104383:104383)</p> <p>Definition of non-COVID cases: single RT-PCR negative</p> <p>Genetic target(s): E gene</p> <p>Samples used: NP swabs, same as for index test</p> <p>Timing of reference standard: not stated</p> <p>Blinded to index test: not stated</p> <p>Incorporated index test: no</p>
Flow and timing	<p>Time interval between index and reference tests: not stated but implies that both tests undertaken in laboratory soon after sample collection</p> <p>All participants received same reference standard: yes</p> <p>Missing data: none reported</p> <p>Uninterpretable results: 3 invalid results were re-tested; 1 positive and 2 negative</p> <p>Indeterminate results (index test): 1 known RT-PCR-positive sample that showed a faint positive test line was re-tested and again showed the same faint test line (considered positive)</p> <p>Indeterminate results (reference standard): none reported</p> <p>Unit of analysis: refers to participants</p>
Comparative	
Notes	<p>Funding: study authors report no specific funding</p> <p>Publication status: preprint</p>

Hogan 2020 (Continued)

Source: medRxiv

Author COI: authors declare no COI present

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	Unclear		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		Unclear risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (Antigen tests)			
DOMAIN 2: Index Test (Rapid PCR tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
Reference standard does not incorporate result of index test?	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk	

Hogan 2020 (Continued)

Are there concerns that the target condition as defined by the reference standard does not match the question?

High

DOMAIN 4: Flow and Timing

Was there an appropriate interval between index test and reference standard? Yes

Did all patients receive the same reference standard? Yes

Were all patients included in the analysis? Unclear

Did all participants receive a reference standard? Yes

Were results presented per patient? Yes

Could the patient flow have introduced bias?

Unclear risk

Lambert-Niclot 2020
Study characteristics

Patient Sampling	<p>Single-group study to estimate sensitivity and specificity: - samples submitted for RT-PCR testing (n = 138)</p> <p>Recruitment: not stated</p> <p>Prospective or retrospective: unclear; testing conducted prospectively</p> <p>Number of samples (samples with confirmed SARS-CoV-2): 138 (94)</p>
Patient characteristics and setting	<p>Setting: not stated</p> <p>Location: samples collected from virology laboratories of 3 university hospital groups from Assistance-Publique-Hôpitaux de Paris (APHP), (Saint-Antoine-Tenon-Trousseau, Saint-Louis-Lariboisière and Kremlin Bicêtre-Paul Brousse)</p> <p>Country: France</p> <p>Dates: 1-15 April 2020</p> <p>Symptoms and severity: not stated</p> <p>Demographics: not stated</p> <p>Exposure history: not stated</p>
Index tests	<p>Test name: COVID-19 Ag Respi-Strip CORIS (no product code)</p> <p>Manufacturer: BioConcept, Gembloux, Belgium</p> <p>Antigen target: SARS-CoV-2 NP</p> <p>Antibody: monoclonal antibodies</p>

Lambert-Niclot 2020 (Continued)

	<p>Test method: CGIA</p> <p>Samples used: NP swabs in VTM (collection process not described)</p> <p>Transport media: either of: COPAN UTM 3 mL, Virocult 1 mL, Eswab Amies 1 mL, 4MRT 3 mL, 0.9% NaCl buffer and cobas ROCHE</p> <p>Sample storage: no cooling or freezing step used</p> <p>Test operator: not stated; presume laboratory staff</p> <p>Definition of test positivity: not stated; as per manufacturer</p> <p>Blinding reported: not stated</p> <p>Timing of samples: not stated; presume on presentation</p>
Target condition and reference standard(s)	<p>Reference standard: RT-PCR (different kits used including RealStar Altona®, Anato-lia®, cobas 6800 Roche®, Allplex™ 2019-nCoV Assay Seegene®)</p> <p>Definition of non-COVID cases: single negative PCR</p> <p>Genetic target(s): E gene</p> <p>Samples used: NP swabs (same as for index)</p> <p>Timing of reference standard: within a few hours after collection; time post onset of symptoms not reported</p> <p>Blinded to index test: unclear</p> <p>Incorporated index test: no</p>
Flow and timing	<p>Time interval between index and reference tests: same sample, both tests conduct-ed within a few hours</p> <p>All participants received same reference standard: yes (different kits)</p> <p>Missing data: none reported</p> <p>Uninterpretable results: 4 samples collected in cobas VTM gave invalid results and all samples in cobas medium were excluded</p> <p>Indeterminate results (index test): control lines reported as "barely visible" for 9 positive and 8 negative tests</p> <p>Indeterminate results (reference standard): none reported</p> <p>Unit of analysis: not reported, but samples tested on day of collection so considered to be 1 per participant</p>
Comparative	
Notes	<p>Funding: no funding sources reported</p> <p>Publication status: accepted manuscript</p> <p>Source: Journal of Clinical Microbiology</p> <p>Author COI: no conflict of interest statement reported</p>

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
------	--------------------	--------------	------------------------

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Lambert-Niclot 2020 (Continued)

DOMAIN 1: Patient Selection

Was a consecutive or random sample of patients enrolled? Unclear

Was a case-control design avoided? Yes

Did the study avoid inappropriate exclusions? Unclear

Did the study avoid inappropriate inclusions? Unclear

Could the selection of patients have introduced bias? Unclear risk

Are there concerns that the included patients and setting do not match the review question? Unclear

DOMAIN 2: Index Test (Antigen tests)

Were the index test results interpreted without knowledge of the results of the reference standard? Unclear

If a threshold was used, was it pre-specified? Yes

Could the conduct or interpretation of the index test have introduced bias? Unclear risk

Are there concerns that the index test, its conduct, or interpretation differ from the review question? Unclear

DOMAIN 2: Index Test (Rapid PCR tests)
DOMAIN 3: Reference Standard

Is the reference standards likely to correctly classify the target condition? No

Were the reference standard results interpreted without knowledge of the results of the index tests? Unclear

Reference standard does not incorporate result of index test? Yes

Could the reference standard, its conduct, or its interpretation have introduced bias? High risk

Are there concerns that the target condition as defined by the reference standard does not match the question? High

DOMAIN 4: Flow and Timing

Lambert-Niclot 2020 (Continued)

Was there an appropriate interval between index test and reference standard?	Yes
Did all patients receive the same reference standard?	Yes
Were all patients included in the analysis?	No
Did all participants receive a reference standard?	Yes
Were results presented per patient?	Yes
Could the patient flow have introduced bias?	High risk

Lieberman 2020
Study characteristics

Patient Sampling	<p>Single-group study to estimate sensitivity and specificity: - samples submitted for clinical diagnostic testing (n = 169; not all samples analysed for all tests)</p> <p>Recruitment: not stated</p> <p>Prospective or retrospective: retrospective (residual samples)</p> <p>Number of samples (samples with confirmed SARS-CoV-2): 169 (87)</p>
Patient characteristics and setting	<p>Setting: not stated; sampled from laboratory</p> <p>Location: Washington State Public Health Laboratory</p> <p>Country: USA</p> <p>Dates: not stated</p> <p>Symptoms and severity: not stated</p> <p>Demographics: not stated</p> <p>Exposure history: not stated</p>
Index tests	<p>Test name: Xpert Xpress</p> <p>Manufacturer: Cepheid</p> <p>Antigen target: E, N2</p> <p>Antibody: N/A</p> <p>Test method: rapid PCR</p> <p>Samples used: NP swabs (collection not described)</p> <p>Transport media: 300 µL of VTM sample</p> <p>Sample storage: all same-sample comparisons were performed on specimens stored at 4 °C for < 72 h with no freeze-thaws</p>

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Lieberman 2020 (Continued)

	<p>Test operator: not stated; presume laboratory staff</p> <p>Common panel of 26 specimens tested at UW by the UW CDC EUA-based LDT or at Lab-Corp Seattle</p> <p>Definition of test positivity: 1 of 2 targets detected was considered positive for all assays; Xpert Xpress data extracted as per IFU definition (positive = both targets or N gene positive; E-gene-positive requires retest)</p> <p>Blinding reported: not stated</p> <p>Timing of samples: not stated</p> <p>Also evaluates: [B] Hologic Panther Fusion RUO, [C] Hologic Panther Fusion EUA, [D] Diasorin Simplexa, [E] Roche cobas 6800</p> <p>in same 26 samples and in additional residual specimens (n = 115) at UW (different N per test)</p>
Target condition and reference standard(s)	<p>Reference standard: RT-PCR; UW CDC EUA-based in-house test (positive if 1 of 2 targets detected - presume at < 40 Ct)</p> <p>Definition of non-COVID cases: single negative PCR</p> <p>Genetic target(s): NI, N2</p> <p>Samples used: NP swabs, as for index test</p> <p>Timing of reference standard: not stated</p> <p>Blinded to index test: not stated</p> <p>Incorporated index test: no</p>
Flow and timing	<p>Time interval between index and reference tests: all testing conducted within 72 h</p> <p>All participants received same reference standard: yes</p> <p>Missing data: none reported; review team excluded data for 28 specimens comparing Panther Fusion with DiaSorin Simplexa</p> <p>Uninterpretable results: not stated</p> <p>Indeterminate results (index test): 'Inconclusive' results (i.e. 1 genetic target detected) were considered positive due to the high specificity of all assays and limited cross-reactivity seen for SARS-CoV-2 primer sets. For Xpert Xpress only 12/13 were positive according to IFU specifications on first test (both targets present, or N gene positive); on retesting the presumptive positive became positive (detection of E-gene but not N-gene)</p> <p>Indeterminate results (reference standard): as for index test</p> <p>Unit of analysis: not stated, only refers to samples</p>
Comparative	
Notes	<p>Funding: no funding statement reported</p> <p>Publication status: accepted manuscript</p> <p>Source: Journal of Clinical Microbiology</p> <p>Author COI: no COI statement reported</p>

Methodological quality

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Lieberman 2020 (Continued)

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	Yes		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		Unclear risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (Antigen tests)			
DOMAIN 2: Index Test (Rapid PCR tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Unclear
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
Reference standard does not incorporate result of index test?	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk	

Lieberman 2020 (Continued)

Are there concerns that the target condition as defined by the reference standard does not match the question?

High

DOMAIN 4: Flow and Timing

Was there an appropriate interval between index test and reference standard? Yes

Did all patients receive the same reference standard? Yes

Were all patients included in the analysis? Unclear

Did all participants receive a reference standard? Yes

Were results presented per patient? Unclear

Could the patient flow have introduced bias?

Unclear risk

Loeffelholz 2020
Study characteristics

Patient Sampling 2-group study to estimate sensitivity and specificity for diagnosis of active disease
- suspected patients referred for COVID-19 testing at 7 sites according to the local criteria (n = 486); sampled to enrich for RT-PCR-positive specimens (not further described)

Recruitment: convenience (in addition, 1 site (LAC+USC) tested specimens from a 4-day point prevalence survey of patients presenting with COVID-19 symptoms)

Prospective or retrospective: retrospective

Number of samples (samples with confirmed SARS-CoV-2): 486 (220)

Patient characteristics and setting Setting: not stated

Location: 7 sites:
Johns Hopkins University, Baltimore;
LAC+USC Medical Centre, University of Southern California, Los Angeles;
Manchester University NHS Foundation Trust Manchester;
Mondor Hospital, Paris;
New York City Dept. Health and Mental Hygiene, NYC;
Niguarda Hospital, Milan;
University Hospital, Newark.

Country: USA, UK, France, Italy

Dates: 1 March-2 April 2020

Symptoms and severity: not stated

Demographics: adults at all sites except New York City Dept. Health and Mental Hygiene and Niguarda Hospital where all age groups were tested (ages not stated)

Exposure history: not stated

Loeffelholz 2020 (Continued)

Index tests	<p>Test name: Cepheid Xpert Xpress SARS-CoV-2 (RUO version, no product code reported)</p> <p>Manufacturer: Cepheid Europe</p> <p>Antigen target: nucleocapsid gene (N2) and the envelope gene (E) (RUO version also detects RdRp gene but this does not contribute to definition of positive)</p> <p>Antibody: N/A</p> <p>Test method: automated point-of-care PCR</p> <p>Samples used: swabs (NP (n = 339), OP (n = 15), combined NP/OP in the same transport vial (n = 97)), and TA (n = 30):</p> <ol style="list-style-type: none"> 1. Baltimore - 61 NP 2. Los Angeles - 88 NP 3. Manchester - 54 NP/OP, 11 NP 4. Paris - 68 NP 5. NYC - NP 11, OP 15, TA 30, NP/OP 43 6. Milan - 79 NP 7. Newark - 21 NP <p>Transport media: VTM (swabs), diluted in saline (TA). 1 site (Manchester) pretreated specimens with an equal volume (≥ 30-< 50% (w/w)) of a guanidine hydrochloride buffer and heated at 80 °C</p> <p>Sample storage: stored at -80 °C prior to index test, except at 1 site (University Hospital, Newark) where specimens were tested in real time, within 2 h by the Xpert test (n = 21).</p> <p>Test operator: not stated; presume laboratory staff</p> <p>Definition of test positivity: as per manufacturer: if both targets are detected, or if only N2 is detected, the test reports a positive result. If only the E target is detected the test reports a presumptive positive result "because this target is shared among some members of the sarbecovirus subgenus of coronaviruses". The RUO version of the test shows the amplification curves and PCR cycle threshold for all 3 genetic targets. The study reports that "The EUA test version cartridge contains the same reagents as the RUO cartridge. The only difference between the tests is the software which in the EUA version allows the user to see amplification curves and results for the N2 and E targets only".</p> <p>Blinding reported: not stated</p> <p>Timing of samples: not stated, presume on presentation</p>
Target condition and reference standard(s)	<p>Reference standard: RT-PCR (sites using each kit not reported, added by review team based on number of samples per site and per RT-PCR kit)</p> <ol style="list-style-type: none"> 1. New York SARS-CoV-2 Real-time Reverse Transcriptase (RT)- PCR Diagnostic Panel; NYC 2. Quest SARS-CoV-2 rRT-PCR (Quest Diagnostics, San Juan Capistrano, US); Los Angeles 3. RealStar® SARS-CoV-2 RT-PCR Kit 1.0 (Altona Diagnostics, Hamburg, Germany); Baltimore and Paris 4. GeneFinder COVID-19 Plus RealAmp Kit (ELITechGroup, Puteaux, France); Milan 5. Allplex 2019-nCoV Assay (Seegene, Seoul, SK); Milan 6. Charité Virology (Berlin, Germany) (in-house); Manchester 7. Abbott RealTime SARS-CoV-2 Assay (Abbott, Des Plaines, US); Newark 8. Simplexa COVID-19 Direct (DiaSorin, Cypress, US); Newark <p>Definition of non-COVID cases: yes (performed prior to index test)</p> <p>Genetic target(s): different targets depending on RT-PCR test used:</p> <ol style="list-style-type: none"> 1. New York Panel; N (N1, N2) 2. Quest; N (N1, N3) 3. RealStar ; S, E

Loeffelholz 2020 (Continued)

4. GeneFinderTM; RdRp, E, N
5. Allplex ; RdRp, E, N
6. Charité Virology; RdRp
7. Abbott RealTime ; RdRp, N
8. Simplexa; ORF1ab, S

Tie-breaker methods (for discrepant results), included: Hologic Panther Fusion (San Diego, USA), Tib-Molbiol LightMix Modular Wuhan Coronavirus E-gene RT-PCR (Roche, Basel, Switzerland); and the CDC assay (IDT primers and probes)

Samples used: as for index test

Timing of reference standard: as for index test

Blinded to index test: no storage; tested in real time

Incorporated index test: no

Flow and timing

Time interval between index and reference tests: same samples but index performed after frozen storage for undefined period of time except at University Hospital, Newark where specimens were tested in real time, within 2 h by the Xpert test

All participants received same reference standard: no

Missing data: 4 Xpert Xpress test results were lost permanently due to a single instrument computer malfunction

Uninterpretable results: 1 Xpert Xpress test was invalid due to a cartridge error (inadequate sample volume)

Indeterminate results (index test) presumptive positive results on Xpert Xpress were not reanalysed by Xpert Xpress, but all discrepant results were reanalysed by a third RT-PCR method

Indeterminate results (reference standard): specimens with inconclusive results by a test, and those with discrepant results between Xpert and the RT-PCR tests were analysed by a third RT-PCR method

1 FN result was inconclusive on Quest SARS-CoV-2, and negative on CDC RT-PCR; re-considered as TN

Of 11 FPs (including 1 presumptive positive on Xpert Xpress), 2 were negative on both New York SARS-CoV-2 and Panther Fusion (remained as FPs), and 9 were negative on in-house RT-PCR but positive on Roche RT-PCR (reclassified as TP)

In addition, 12 specimens (8 NP, 4 NP/OP) were inconclusive by the NY (RT)- PCR Diagnostic Panel and considered positive for data analysis purposes in the study. Of these, 11 were positive by the Xpert test and 1 was presumptive positive (EUA version of Xpert test). In 4 of these only the N1 target was detected and in 8 only the N2 target was detected by the New York EUA method, all with Ct values > 36

One NP specimen was inconclusive by the Quest SARS-CoV-2 rRT-PCR test and negative by the Xpert test. The Quest test reports inconclusive if only a single target (N1 or N3) is detected. They were unable to determine which target was detected by the Quest test. This specimen was negative by a tie-breaker NAAT.

Unit of analysis: not stated; only samples reported

Comparative

Notes

Funding: not stated; presume funded by test manufacturer (see COI statement)

Publication status: accepted manuscript

Source: Journal of Clinical Microbiology

Author COI: the study was designed and supervised by the sponsor, Cepheid. Data were collected by investigators at each study site, and statistical analyses were performed by a Cepheid author. Cepheid authors wrote the first draft of the manuscript. All study authors vouch for the accuracy and completeness of the data reported.

Methodological quality

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Loeffelholz 2020 (Continued)

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	No		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Yes		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (Antigen tests)			
DOMAIN 2: Index Test (Rapid PCR tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Unclear		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 3: Reference Standard			

Loeffelholz 2020 (Continued)

Is the reference standard likely to correctly classify the target condition?	No	
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes	
Reference standard does not incorporate result of index test?	Yes	
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk
Are there concerns that the target condition as defined by the reference standard does not match the question?		High
DOMAIN 4: Flow and Timing		
Was there an appropriate interval between index test and reference standard?	Yes	
Did all patients receive the same reference standard?	Yes	
Were all patients included in the analysis?	No	
Did all participants receive a reference standard?	Yes	
Were results presented per patient?	Yes	
Could the patient flow have introduced bias?		High risk

Mertens 2020

Study characteristics

Patient Sampling	<p>Single-group study to estimate sensitivity and specificity for diagnosis of active disease: - samples from patients suspected of SARS-CoV-2 infections (n = 328)</p> <p>Recruitment: random sampling of samples submitted to 3 laboratories 322/328 NP samples (NP swabs) were randomly selected</p> <p>Prospective or retrospective: retrospectively</p> <p>Number of samples (samples with confirmed SARS-CoV-2): 328 (132)</p>
Patient characteristics and setting	<p>Setting: unclear; samples from university laboratories (discussion states that no outpatient population has been sampled, therefore assume inpatients and HCW samples)</p> <p>Location: laboratories at Université Libre de Bruxelles (LHUB-ULB), UZ Leuven and Centre Hospitalier Universitaire Sart-Tilman (CHU) Liège</p> <p>Country: Belgium</p> <p>Dates: 19-30 March 2020</p> <p>Symptoms and severity: not reported</p> <p>Demographics: not reported</p> <p>Exposure history: unclear; 53/328 samples were from HCW</p>
Index tests	<p>Test name: COVID-19 Ag Respi-Strip</p> <p>Manufacturer: Coris BioConcept (Belgium)</p> <p>Antigen target: SARS-CoV and SARS-CoV-2 highly conserved nucleoprotein</p> <p>Antibody: monoclonal antibodies directed against SARS-CoV and SARS-CoV-2 highly conserved nucleoprotein antigen</p> <p>Test method: immunochromatographic assay using colloidal gold (CGIA)</p> <p>Samples used: remnant respiratory specimens (322 NP swabs, 4 NP aspirate and 2 BAL)</p> <p>Transport media: NP: flocculated swab + UTM 3 mL (or 1 mL of Amies) (Copan, Brescia, Italy); NPA: 3 mL VTM (veal infusion broth (Difco, Becton Dickinson, Sparks, MD, USA) supplemented with bovine albumin (Sigma Aldrich, St Louis, MO, USA)) BAL: N/A</p> <p>Sample storage: not described</p> <p>Test operator: laboratory technician</p> <p>Definition of test positivity: visible reddish-purple band appearing at the Test line position (T)</p> <p>Blinding reported: not stated</p> <p>Timing of samples: not clear</p>
Target condition and reference standard(s)	<p>Reference standard: qRT-PCR: RealStar SARS-CoV-2 RT-PCR Kit from Altona-diagnostics with a cut-off set at 40 Ct (LHUB-ULB); Roche LC480 thermocycler using Taqman Fast Virus 1-Step Master Mix (Thermo Fisher) (Liege); QuantStudio Dx (Thermo Fisher Scientific) or Panther Fusion (PF, Hologic, San Diego, USA) (UZ Leuven)</p> <p>Definition of non-COVID cases:</p> <ul style="list-style-type: none"> Genetic target(s): RealStar: not stated;

Mertens 2020 (Continued)

- Taqman Fast Virus: RdRp and E genes
- QuantStudio Dx; "slightly adapted" E-gene
- Panther Fusion: E gene and ORF1-ab

Samples used: as for index test (respiratory specimens (322 NP swabs, 4 NP aspirate and 2 BAL)

Timing of reference standard: not stated; same samples as for index test but analysed at time of collection

Blinded to index test: yes (undertaken for diagnostic purposes at time of collection)

Incorporated index test: no

Flow and timing

Time interval between index and reference tests: same samples used; discussion report 'some delay' between PCR and antigen testing

All participants received same reference standard: yes but different RT-PCR kits

Missing data: no

Uninterpretable results: none reported; discussion reports some difficulties in visualising the strip through the closed tube requiring the lab technician to open the test tube in the laminar air flow cabinet and pull out the strip with forceps

Indeterminate results (index test): weak T lines considered positive

Indeterminate results (reference standard): none reported; sensitivity can be extracted for cases with Ct values < or > 25 (high vs lower viral load)

Unit of analysis: refers to participants

Comparative
Notes

Funding: not stated

Publication status: preprint (not peer-reviewed)

Sourcepreprint server (medRxiv)

Author COI: the IVD medical device has been developed by the investigator Pascal Mertens, Henri Magein, and Justine Bouzet working for Coris BioConcept (potential conflict of interest declared even though they don't have any share in this company); Thierry Leclipteux was involved in the development of this test and is the CEO of Coris Bioconcept (potential conflict of interest declared). All scientific investigators that are external to Coris BioConcept declare having no conflict of interest.

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Yes		
Was a case-control design avoided?	Yes		
Did the study avoid inappropriate exclusions?	Yes		

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Mertens 2020 (Continued)

Did the study avoid inappropriate inclusions? Yes

Could the selection of patients have introduced bias? Low risk

Are there concerns that the included patients and setting do not match the review question? High

DOMAIN 2: Index Test (Antigen tests)

Were the index test results interpreted without knowledge of the results of the reference standard? Unclear

If a threshold was used, was it pre-specified? Yes

Could the conduct or interpretation of the index test have introduced bias? Unclear risk

Are there concerns that the index test, its conduct, or interpretation differ from the review question? High

DOMAIN 2: Index Test (Rapid PCR tests)
DOMAIN 3: Reference Standard

Is the reference standards likely to correctly classify the target condition? No

Were the reference standard results interpreted without knowledge of the results of the index tests? Unclear

Reference standard does not incorporate result of index test? Yes

Could the reference standard, its conduct, or its interpretation have introduced bias? High risk

Are there concerns that the target condition as defined by the reference standard does not match the question? High

DOMAIN 4: Flow and Timing

Was there an appropriate interval between index test and reference standard? Yes

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Mertens 2020 (Continued)

Did all patients receive the same reference standard?	Yes
Were all patients included in the analysis?	Yes
Did all participants receive a reference standard?	Yes
Were results presented per patient?	Yes
Could the patient flow have introduced bias?	Low risk

Mitchell 2020
Study characteristics

Patient Sampling	<p>Single-group study to estimate sensitivity and specificity for diagnosis of active disease: - samples positive and negative on 1 of 2 SARS-CoV-2 RT-PCR assays</p> <p>Recruitment: not stated; suggests possible deliberate sampling of positive cases</p> <p>Prospective or retrospective: retrospective (residual samples)</p> <p>Number of samples (samples with confirmed SARS-CoV-2): 61 (46)</p>
Patient characteristics and setting	<p>Setting: not stated; 2 independent laboratories (Class II biosafety cabinet (BSC))</p> <p>Location: not stated; author institutions University of Pittsburgh School of Medicine, Pittsburgh and Laboratory of Viral Diseases, Wadsworth Centre, New York State Department of Health, Albany, NY</p> <p>Country: USA</p> <p>Dates: not stated</p> <p>Symptoms and severity: not stated</p> <p>Demographics: not stated</p> <p>Exposure history: not stated</p>
Index tests	<p>Test name: ID NOW COVID-19 (product code not reported)</p> <p>Manufacturer: Abbott, Chicago, USA</p> <p>Antigen target: not stated</p> <p>Antibody: N/A</p> <p>Test method: not stated (should be isothermal PCR)</p> <p>Samples used: NP samples (residual samples)</p> <p>Transport media: VTM; no further detail (no longer covered on IFU)</p> <p>Sample storage: stored at -80 °C prior to testing</p>

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Mitchell 2020 (Continued)

	Test operator: certified laboratory personnel Definition of test positivity: not stated; as per manufacturer Blinding reported: not stated Timing of samples: not stated
Target condition and reference standard(s)	Reference standard: CDC EUA or the New York EUA RT-PCR assays Definition of non-COVID cases: single RT-PCR negative Genetic target(s): not stated Samples used: as for index test Timing of reference standard: as for index test Blinded to index test: not stated; samples analysed at or near time of collection Incorporated index test: no
Flow and timing	Time interval between index and reference tests: same samples but used at different times (samples used for index test stored at -80 °C) All participants received same reference standard: no, either the CDC EUA or the New York EUA assays Missing data: none reported Uninterpretable results: none reported Indeterminate results (index test): none reported Indeterminate results (reference standard): none reported Unit of analysis: not stated; only samples reported
Comparative	
Notes	Funding: not stated Publication status: accepted manuscript Source: Journal of Clinical Virology Author COI: COI not mentioned by study authors

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	Yes		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Mitchell 2020 (Continued)

Could the selection of patients have introduced bias?	Unclear risk
Are there concerns that the included patients and setting do not match the review question?	High
DOMAIN 2: Index Test (Antigen tests)	
DOMAIN 2: Index Test (Rapid PCR tests)	
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear
If a threshold was used, was it pre-specified?	Yes
Could the conduct or interpretation of the index test have introduced bias?	Unclear risk
Are there concerns that the index test, its conduct, or interpretation differ from the review question?	High
DOMAIN 3: Reference Standard	
Is the reference standards likely to correctly classify the target condition?	No
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes
Reference standard does not incorporate result of index test?	Yes
Could the reference standard, its conduct, or its interpretation have introduced bias?	High risk
Are there concerns that the target condition as defined by the reference standard does not match the question?	High
DOMAIN 4: Flow and Timing	
Was there an appropriate interval between index test and reference standard?	Yes
Did all patients receive the same reference standard?	Yes
Were all patients included in the analysis?	Unclear
Did all participants receive a reference standard?	Yes
Were results presented per patient?	Unclear
Could the patient flow have introduced bias?	Unclear risk

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Moore 2020

Study characteristics

Patient Sampling	<p>2-group study to estimate sensitivity and specificity: - samples from symptomatic (fever or cough or shortness of breath) adult and paediatric outpatients, ED patients, and inpatients</p> <p>Recruitment: consecutive (first 94 participants), then all PCR-positive samples plus the next PCR-negative sample after each positive sample, to a total of 200 samples</p> <p>Prospective or retrospective: retrospective (participant and sample details extracted from the electronic medical record)</p> <p>Number of samples (samples with confirmed SARS-CoV-2): 200 (125)</p>
Patient characteristics and setting	<p>Setting: mixed (outpatients, ED patients and inpatients)</p> <p>Location: Rush University Medical Centre (RUMC) or Rush Oak Park Hospital (ROPH), Chicago</p> <p>Country: USA</p> <p>Dates: 27 March-9 April 2020</p> <p>Symptoms and severity: 79 (39.5%) hospitalised including 29 in ICU, 76 (38%) ambulatory care including 55 seen in a designated COVID-19 screening clinic), and 45 (23%) seen at ED</p> <p>Demographics: mean age 50 years (SD 17 years), 92 (46%) men</p> <p>Exposure history: not stated</p>
Index tests	<p>Test name: ID NOW (no product code)</p> <p>Manufacturer: Abbott</p> <p>Antigen target: RdRp</p> <p>Antibody: N/A</p> <p>Test method: rapid PCR (isothermal)</p> <p>Samples used: NP swabs in 3 mL VTM (collection not reported)</p> <p>Transport media: M4-RT VTM (Remel, Lenexa, KS)</p> <p>Sample storage: stored at 4 °C if all testing could not be completed on the same day; all tests completed within 72 h of collection</p> <p>Test operator: not stated; presume laboratory staff</p> <p>Definition of test positivity: as per manufacturer</p> <p>Blinding reported: not stated</p> <p>Timing of samples: not stated; presumably on presentation but no information on symptom status</p>
Target condition and reference standard(s)	<p>Reference standard: RT-PCR; 2 methods used in the study</p> <ol style="list-style-type: none"> 1. modified CDC RT-PCR (positive result required Ct < 40 for both targets; negative if neither target detected and positive amplification curve for control (RP) gene; inconclusive if only 1 target detected at Ct < 40, and test repeated)

Moore 2020 (Continued)

2. Abbott RealTime SARS-CoV-2 RT-PCR (amplification curves reported as detected or not detected)

Record review used to verify status of 8 samples positive on RealTime assay and negative (6) or inconclusive (2) on CDC assay (all considered disease-positive)

Definition of non-COVID cases: single RT-PCR negative

Genetic target(s):

1. N1, N2
2. N, RdRp

Samples used: NP swabs in VTM, as for index test

Timing of reference standard: not stated

Blinded to index test: not stated

Incorporated index test: no

Flow and timing

Time interval between index and reference tests: all 3 tests conducted within 72 h of sample collection

All participants received same reference standard: no? (all received both RT-PCR tests, only discordant results on RT-PCR had record review)

Missing data: none reported

Uninterpretable results: 2 results were invalid on ID NOW and were not retested (excluded)

Indeterminate results (index test): none reported

Indeterminate results (reference standard): discordant results between 2 RT-PCR assays had record review to determine presence/absence COVID-19 infection

Unit of analysis: participants (specimens from 200 unique participants)

Comparative
Notes

Funding: none reported (some reagents supplied from NIH)

Publication status: preprint

Source: medRxiv

Author COI: no COI statement was reported

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	No		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		

Moore 2020 (Continued)

Did the study avoid inappropriate inclusions?	Yes
Could the selection of patients have introduced bias?	High risk
Are there concerns that the included patients and setting do not match the review question?	High
DOMAIN 2: Index Test (Antigen tests)	
DOMAIN 2: Index Test (Rapid PCR tests)	
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear
If a threshold was used, was it pre-specified?	Yes
Could the conduct or interpretation of the index test have introduced bias?	Unclear risk
Are there concerns that the index test, its conduct, or interpretation differ from the review question?	High
DOMAIN 3: Reference Standard	
Is the reference standards likely to correctly classify the target condition?	Yes
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear
Reference standard does not incorporate result of index test?	Yes
Could the reference standard, its conduct, or its interpretation have introduced bias?	Unclear risk
Are there concerns that the target condition as defined by the reference standard does not match the question?	Low concern
DOMAIN 4: Flow and Timing	
Was there an appropriate interval between index test and reference standard?	Yes

Moore 2020 (Continued)

Did all patients receive the same reference standard?	Yes
Were all patients included in the analysis?	No
Did all participants receive a reference standard?	Yes
Were results presented per patient?	Yes
Could the patient flow have introduced bias?	High risk

Moran 2020
Study characteristics

Patient Sampling	<p>Single-group study to estimate sensitivity and specificity: - specimens collected from inpatients and ambulatory patients at the University of Chicago</p> <p>Recruitment: not stated</p> <p>Prospective or retrospective: not stated</p> <p>Number of samples (samples with confirmed SARS-CoV-2): 103 (42)</p>
Patient characteristics and setting	<p>Setting: inpatient and ambulatory; samples selected from central laboratory</p> <p>Location: Clinical Microbiology Laboratory, University of Chicago</p> <p>Country: USA</p> <p>Dates: not stated</p> <p>Symptoms and severity: not stated</p> <p>Demographics: not stated</p> <p>Exposure history: not stated</p>
Index tests	<p>Test name: Xpert Xpress SARS-CoV-2 assay (no product code)</p> <p>Manufacturer: Cepheid, Sunnyvale, CA</p> <p>Antigen target: E, N (N2 region)</p> <p>Antibody: N/A</p> <p>Test method: rapid PCR</p> <p>Samples used: 8 nasal and 95 NP swabs</p> <p>Transport media: none described</p> <p>Sample storage: not stated</p> <p>Test operator: not stated; presume laboratory staff</p>

Moran 2020 (Continued)

	<p>Definition of test positivity: not stated; re-testing using Xpert Xpress was undertaken for an N-gene positive result due to discrepancy with RT-PCR (not in line with IFU recommendation)</p> <p>Blinding reported: not stated</p> <p>Timing of samples: not stated</p>
Target condition and reference standard(s)	<p>Reference standard: Roche cobas SARS-CoV-2 assay on the cobas 6800 system (Roche Molecular Systems, Branchburg, NJ)</p> <p>Definition of non-COVID cases: single RT-PCR negative</p> <p>Genetic target(s): ORF1, E</p> <p>Samples used: nasal and NP swabs; same as for index test</p> <p>Timing of reference standard: not stated</p> <p>Blinded to index test: not stated</p> <p>Incorporated index test: no</p>
Flow and timing	<p>Time interval between index and reference tests: not stated; same sample and appear to have both been conducted soon after sample collection</p> <p>All participants received same reference standard: yes</p> <p>Missing data: none reported</p> <p>Uninterpretable results: none reported</p> <p>Indeterminate results (index test): single FP (negative on E gene and low positive on N gene) was retested with Xpert Xpress and considered negative on both targets</p> <p>Indeterminate results (reference standard): single FP was retested on RT-PCR and found to be repeatedly negative</p> <p>Unit of analysis: refers to participants</p>
Comparative	
Notes	<p>Funding: none described</p> <p>Publication status: accepted manuscript</p> <p>Source: Journal of Clinical Microbiology</p> <p>Author COI: no COI statement was reported</p>

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	Yes		

Moran 2020 (Continued)

Did the study avoid inappropriate exclusions?	Unclear
Did the study avoid inappropriate inclusions?	Unclear
Could the selection of patients have introduced bias?	Unclear risk
Are there concerns that the included patients and setting do not match the review question?	Unclear
DOMAIN 2: Index Test (Antigen tests)	
DOMAIN 2: Index Test (Rapid PCR tests)	
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear
If a threshold was used, was it pre-specified?	No
Could the conduct or interpretation of the index test have introduced bias?	High risk
Are there concerns that the index test, its conduct, or interpretation differ from the review question?	Unclear
DOMAIN 3: Reference Standard	
Is the reference standards likely to correctly classify the target condition?	No
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear
Reference standard does not incorporate result of index test?	Yes
Could the reference standard, its conduct, or its interpretation have introduced bias?	Unclear risk
Are there concerns that the target condition as defined by the reference standard does not match the question?	High
DOMAIN 4: Flow and Timing	
Was there an appropriate interval between index test and reference standard?	Yes
Did all patients receive the same reference standard?	Yes
Were all patients included in the analysis?	Unclear
Did all participants receive a reference standard?	Yes

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Moran 2020 (Continued)

Were results presented per patient? Yes

Could the patient flow have introduced bias? Unclear risk

Porte 2020

Study characteristics

Patient Sampling

2-group study to estimate sensitivity and specificity for diagnosis of active disease:
- samples from suspected COVID-19 cases (n = 1453) with deliberate sampling of PCR-positive and negative cases on a 2:1 basis (n = 127)

Recruitment: convenience sampling

Prospective or retrospective: retrospectively

Number of samples (samples with confirmed SARS-CoV-2): 127 (82)

Patient characteristics and setting

Setting: outpatients attending ED at private medical centre (hospital)

Location: Clínica Alemana, Santiago

Country: Chile

Dates: 16-21 March 2020

Symptoms and severity: cough 94 (74.6%)
Fever 77 (61.1%)
Median duration of symptoms of 2 days (IQR 1-4; range 0-12)
Duration of symptoms: day 0-3 91 (72.2%); day 4-7 27 (22.4%); day ≥ 8 8 (6.3%)

Demographics: 68 male (53.5%), median age 38 years (IQR 29.5-44; range 1-91)

Exposure history: not stated

Index tests

Test name: diagnostic Kit for 2019-Novel Coronavirus (2019-nCoV) Ag Test (Cat. N° YRLF04401025, lot N° 2002N408)

Manufacturer: Bioeasy Biotechnology Co., Shenzhen, China

Antigen target: SARS-CoV-2 nucleocapsid protein

Antibody: not stated

Test method: FIA

Samples used: remnant (?) OP and NP swabs in 3 mL UTM

Transport media: UTM-RT System, Copan Diagnostics, Murrieta, CA, USA

Sample storage: stored at 4 °C and tested within 48 h

Test operator: laboratory technician

Definition of test positivity: not stated; test "automatically delivers a positive or negative qualitative result"

Positive or negative defined qualitatively

Blinding reported: yes

Timing of samples: on presentation

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Porte 2020 (Continued)

	Within 48 h of the PCR test but it doesn't say when PCR test was performed (median duration of symptoms reported in D9)		
Target condition and reference standard(s)	Reference standard: RT-PCR (COVID-19 Genesig Real-Time PCR assay (Primer Design Ltd., Chandler's Ford, UK)); Ct ≤ 40 considered positive Definition of non-COVID cases: single RT-PCR negative Genetic target(s): not stated Samples used: as for index test; same OP and NP swabs used Timing of reference standard: median 2 d post symptom onset (IQR 1-4; range 0-12) Blinded to index test: yes (index test done within 48 h of PCR test) Incorporated index test: no		
Flow and timing	Time interval between index and reference tests: same sample used; within 48 h All participants received same reference standard: yes Missing data: no Uninterpretable results: not reported Indeterminate results (index test): not reported Indeterminate results (reference standard): not reported Unit of analysis: participants		
Comparative			
Notes	Funding: this work did not receive funding Publication status: preprint (not peer-reviewed) Source: SSRN Author COI: all study authors declare no competing interests		
Methodological quality			
Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	No		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Yes		
Could the selection of patients have introduced bias?		High risk	

Porte 2020 (Continued)

Are there concerns that the included patients and setting do not match the review question? High

DOMAIN 2: Index Test (Antigen tests)

Were the index test results interpreted without knowledge of the results of the reference standard? Yes

If a threshold was used, was it pre-specified? Yes

Could the conduct or interpretation of the index test have introduced bias? Low risk

Are there concerns that the index test, its conduct, or interpretation differ from the review question? High

DOMAIN 2: Index Test (Rapid PCR tests)
DOMAIN 3: Reference Standard

Is the reference standards likely to correctly classify the target condition? No

Were the reference standard results interpreted without knowledge of the results of the index tests? Yes

Reference standard does not incorporate result of index test? Yes

Could the reference standard, its conduct, or its interpretation have introduced bias? High risk

Are there concerns that the target condition as defined by the reference standard does not match the question? High

DOMAIN 4: Flow and Timing

Was there an appropriate interval between index test and reference standard? Yes

Did all patients receive the same reference standard? Yes

Were all patients included in the analysis? Yes

Did all participants receive a reference standard? Yes

Were results presented per patient? Yes

Could the patient flow have introduced bias? Low risk

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Rhoads 2020

Study characteristics

Patient Sampling	<p>Single-group study to estimate sensitivity: - samples positive using standard of care testing (n = 96) (14 negative controls (UTM) included to control for carry-over contamination only)</p> <p>Recruitment: convenience</p> <p>Prospective or retrospective: retrospective (remnant samples)</p> <p>Number of samples (samples with confirmed SARS-CoV-2): 96 (96)</p>
Patient characteristics and setting	<p>Setting: not stated; includes self-collected and provided-collected samples</p> <p>Location: not stated; author institutions University Hospitals Cleveland Medical Centre and Case Western Reserve University</p> <p>Country: USA</p> <p>Dates: not stated</p> <p>Symptoms and severity: not stated</p> <p>Demographics: not stated</p> <p>Exposure history: not stated</p>
Index tests	<p>Test name: ID NOW (product codes not reported)</p> <p>Manufacturer: Abbott; Chicago, USA Also reports evaluation of Diasorin Simplexa (not eligible for this review)</p> <p>Antigen target: not stated</p> <p>Antibody: N/A</p> <p>Test method: isothermal PCR</p> <p>Samples used: nasal swabs (self-collected) and NP swabs (provider collected); all remnant samples</p> <p>Transport media: nasal swabs (2 mL normal saline) and NP swabs (3 mL UTM)</p> <p>Sample storage: not stated</p> <p>Test operator: not stated; presume laboratory staff</p> <p>Definition of test positivity: not stated; as per manufacturer</p> <p>Blinding reported: not stated</p> <p>Timing of samples: not stated</p>
Target condition and reference standard(s)	<p>Reference standard: standard of care testing for original samples; remnant samples re-tested with modified CDC RT-PCR (using 7500 Fast instrument and using alternate RNA extraction method (Maxwell RSC 6 instrument with Viral TNA Kit (Cat# AS1330; Promega, Madison, USA)); samples with 1 positive target detected considered positive instead of "inconclusive"</p> <p>Definition of non-COVID cases: as for index test</p>

Rhoads 2020 (Continued)

Genetic target(s): N1 and N2
 Samples used: as for index test
 Timing of reference standard: as for index test
 Blinded to index test: as for index test
 Incorporated index test: as for index test

Flow and timing	<p>Time interval between index and reference tests: same samples used</p> <p>All participants received same reference standard: yes</p> <p>Missing data: none reported</p> <p>Uninterpretable results: none reported</p> <p>Indeterminate results (index test): none reported</p> <p>Indeterminate results (reference standard): RT-PCR detected only 1 of 2 targets for 2 samples (both considered positive (diagnosed as positive on original sample testing); both were negative on index test)</p> <p>Unit of analysis: not stated; only samples reported</p>		
Comparative			
Notes	<p>Funding: no outside funding used to support the investigation</p> <p>Publication status: accepted manuscript</p> <p>Source: Journal of Clinical Microbiology</p> <p>Author COI: COI not mentioned by study authors</p>		
Methodological quality			
Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	No		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (Antigen tests)			
DOMAIN 2: Index Test (Rapid PCR tests)			

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Rhoads 2020 (Continued)

Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear	
If a threshold was used, was it pre-specified?	Yes	
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk
Are there concerns that the index test, its conduct, or interpretation differ from the review question?		High
DOMAIN 3: Reference Standard		
Is the reference standards likely to correctly classify the target condition?	Yes	
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear	
Reference standard does not incorporate result of index test?	Yes	
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk
Are there concerns that the target condition as defined by the reference standard does not match the question?		High
DOMAIN 4: Flow and Timing		
Was there an appropriate interval between index test and reference standard?	Yes	
Did all patients receive the same reference standard?	Yes	
Were all patients included in the analysis?	Unclear	
Did all participants receive a reference standard?	Yes	
Were results presented per patient?	Unclear	
Could the patient flow have introduced bias?		Unclear risk

Smithgall 2020 [A]

Study characteristics

Patient Sampling	2-group study to estimate sensitivity and specificity:
------------------	--

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Smithgall 2020 [A] (Continued)

	<p>- patients undergoing routine clinical testing by RT-PCR (n = 113)</p> <p>Recruitment: unclear; describes deliberate sampling of samples with high, medium and low Ct values on the reference standard RT-PCR</p> <p>Prospective or retrospective: unclear; residual swabs used but testing undertaken within 48 h of sample collection</p> <p>Number of samples (samples with confirmed SARS-CoV-2): 113 (88)</p>
Patient characteristics and setting	<p>Setting: inpatient and ED (n from each not reported)</p> <p>Location: not stated; author institution is Columbia University Irving Medical Centre</p> <p>Country: USA</p> <p>Dates: 8-13 April 2020</p> <p>Symptoms and severity: not stated</p> <p>Demographics: 111 adult (range 23-101 years; average 65 years for RT-PCR-positive and 43 years for RT-PCR-negative); 2 paediatric (age 1 day and 5 days) 61, 54% male</p> <p>Exposure history: not stated</p>
Index tests	<p>Test name: [A] ID NOW (see Smithgall 2020 [B] for details of comparator test) (product codes not reported)</p> <p>Manufacturer: [A] Abbott</p> <p>Antigen target: [A] RdRp gene</p> <p>Antibody: N/A</p> <p>Test method: [A] isothermal PCR</p> <p>Samples used: residual NP swabs (collection not described)</p> <p>Transport media: 3 mL VTM (M4RT VTM; ThermoFisher Scientific, Waltham, MA) or UTM (UTM; Becton Dickinson and Co., Franklin Lakes, NJ)</p> <p>Sample storage: stored at 4 °C; testing completed within 48 h of sample collection</p> <p>Test operator: not stated; presume laboratory staff</p> <p>Definition of test positivity: automated as per manufacturer</p> <p>Blinding reported: not stated</p> <p>Timing of samples: not stated; presume on admission or presentation at ED</p>
Target condition and reference standard(s)	<p>Reference standard: RT-PCR with cobas SARS-CoV-2 assay on the 6800 platform (Roche Diagnostics, Indianapolis, IN); threshold not stated, all Ct values < 37 on both target genes</p> <p>Definition of non-COVID cases: not stated; presume single RT-PCR negative</p> <p>Genetic target(s): ORF1 a/b, E-gene</p> <p>Samples used: as for index test</p> <p>Timing of reference standard: as for index test</p> <p>Blinded to index test: as for index test</p>

Smithgall 2020 [A] (Continued)

	Incorporated index test: no
Flow and timing	Time interval between index and reference tests: simultaneous; same samples used All participants received same reference standard: yes Missing data: none reported Uninterpretable results: Indeterminate results (index test): Xpert: 1 sample was a presumptive positive based on detection of E-gene target but not the N2 target Indeterminate results (reference standard): none reported Unit of analysis: participants
Comparative	
Notes	Funding: none reported Publication status: published Source: Journal of Clinical Virology Author COI: study authors report no conflicts of interest present

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	No		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (Antigen tests)			
DOMAIN 2: Index Test (Rapid PCR tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	No		

Smithgall 2020 [A] (Continued)

Could the conduct or interpretation of the index test have introduced bias?	High risk
Are there concerns that the index test, its conduct, or interpretation differ from the review question?	High
DOMAIN 3: Reference Standard	
Is the reference standards likely to correctly classify the target condition?	No
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear
Reference standard does not incorporate result of index test?	Yes
Could the reference standard, its conduct, or its interpretation have introduced bias?	High risk
Are there concerns that the target condition as defined by the reference standard does not match the question?	High
DOMAIN 4: Flow and Timing	
Was there an appropriate interval between index test and reference standard?	Yes
Did all patients receive the same reference standard?	Yes
Were all patients included in the analysis?	Unclear
Did all participants receive a reference standard?	Yes
Were results presented per patient?	Yes
Could the patient flow have introduced bias?	Unclear risk

Smithgall 2020 [B]

Study characteristics	
Patient Sampling	See Smithgall 2020 [A] for full study details and QUADAS-2 entries
Patient characteristics and setting	See Smithgall 2020 [A] for full study details and QUADAS-2 entries

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Smithgall 2020 [B] (Continued)

Index tests	<p>Test name: [B] Xpert Xpress (product codes not reported) (see Smithgall 2020 [A] for details of comparator test)</p> <p>Manufacturer: [B] Cepheid</p> <p>Antigen target: [B] N2, E genes</p> <p>Antibody: N/A</p> <p>Test method: [B] automated RT-PCR</p> <p>Samples used: residual NP swabs (collection not described)</p> <p>Transport media: 3 mL VTM (M4RT VTM; ThermoFisher Scientific, Waltham, MA) or UTM (UTM; Becton Dickinson and Co., Franklin Lakes, NJ)</p> <p>Sample storage: stored at 4 °C; testing completed within 48 h of sample collection.</p> <p>Test operator: not stated; presume laboratory staff</p> <p>Definition of test positivity: automated as per manufacturer</p> <p>Blinding reported: not stated</p> <p>Timing of samples: not stated; presume on admission or presentation at ED</p>
Target condition and reference standard(s)	See Smithgall 2020 [A] for full study details and QUADAS-2 entries
Flow and timing	See Smithgall 2020 [A] for full study details and QUADAS-2 entries
Comparative	
Notes	See Smithgall 2020 [A] for full study details and QUADAS-2 entries

Weitzel 2020 [A]

Study characteristics

Patient Sampling	<p>Single-group study to estimate sensitivity and specificity: - samples from patients with respiratory symptoms and/or fever attending a private hospital ED</p> <p>Recruitment: convenience with deliberate sampling of positive cases to ensure a 2:1 distribution reported (5276 samples processed during study period)</p> <p>Prospective or retrospective: retrospective</p> <p>Number of samples (samples with confirmed SARS-CoV-2): 111 (80)</p> <p>*17 samples included in Porte 2020</p>
Patient characteristics and setting	<p>Setting: ED (private hospital)</p> <p>Location: Clínica Alemana de Santiago</p> <p>Country: Chile</p> <p>Dates: 16 March-26 April 2020</p>

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Weitzel 2020 [A] (Continued)

Symptoms and severity: respiratory symptoms and/or fever; no further detail

Demographics: median age 40 years; 50, 45% male (median age 38 years, 43% male for all samples tested during period)

Exposure history: none reported

Index tests

Weitzel 2020 [A] entry is for test [A] in the list below

Test name:

[A] Biocredit COVID-19 Ag One Step SARS-CoV-2 Antigen Test (RapiGEN Inc., Anyang-si, Gyeonggi-do, Republic of Korea)

[B] COVID-19 Antigen Rapid Test Device StrongStep COVID-19 Antigen Test (Liming Bio-Products Co., Jiangsu, China)

[C] Huaketai New Coronavirus (SARS-CoV-2) N Protein Detection Kit (Fluorescence immunochromatography) (Savant Biotechnology Co., Beijing, China),

[D] Diagnostic Kit for 2019-Novel Coronavirus (2019-nCoV) Ag Test (Fluorescence Immunochromatographic Assay) (Bioeasy Biotechnology Co., Shenzhen, China).

Manufacturer:

[A] RapiGEN Inc., Anyang-si, Gyeonggi-do, Republic of Korea

[B] Liming Bio-Products Co., Jiangsu, China

[C] Savant Biotechnology Co., Beijing, China

[D] Bioeasy Biotechnology Co., Shenzhen, China

Antigen target: not reported in study

Antibody: not reported in study

Test method: [A] and [B] CGIA

[C] and [D] FIA

Samples used: NOP swabs in 3 mL UTM

Transport media: UTM-RT System (Copan Diagnostics, Murrieta, CA, USA)

Sample storage: stored at -80 °C; index tests applied on 28 and 29 April 2020

Test operator: single, trained laboratory technician under BSL2 cabinet; visual outputs read by 2 independent observers with referral to third if needed

Definition of test positivity: as per manufacturer; Beijing Savant test required use of manufacturer supplied UV torch due to unavailability of reader device in Chile

Blinding reported: yes; blinding stated

Timing of samples: median 2 days (IQR 1-5 days); 88% (96/109) during the first week of symptoms

Target condition and reference standard(s)

Reference standard: RT-PCR; COVID-19 Genesig Real-Time PCR assay (Primerdesign Ltd., Chandler's Ford, UK). Ct ≤ 40 considered positive

Definition of non-COVID cases: single PCR negative

Genetic target(s): RdRp

Samples used: NOP swabs; as for index

Timing of reference standard: as for index test; median 2 days (IQR 1-5 days)

Blinded to index test: yes; prior to index

Incorporated index test: no

Weitzel 2020 [A] (Continued)

Flow and timing	<p>Time interval between index and reference tests: same samples; index tests conducted after frozen storage</p> <p>All participants received same reference standard: yes</p> <p>Missing data: none reported; evaluation of Liming test was discontinued after initial poor performance (zero TP)</p> <p>Uninterpretable results: 2 tests had invalid results due to insufficient liquid migration (2 results excluded for each test)</p> <p>Indeterminate results (index test): visual interpretation of the Beijing Savant assay (using manufacturer supplied UV torch) was reportedly difficult under daylight conditions; manufacturer's fluorescence reader not available in Chile.</p> <p>Indeterminate results (reference standard): none reported</p> <p>Unit of analysis: participants</p>
Comparative	
Notes	<p>Funding: study authors report that the work received no funding; Savant Biotechnology Co. provided test kits free of charge</p> <p>Publication status: preprint</p> <p>Source: medRxiv</p> <p>Author COI: all authors declare no competing interests</p>

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	No		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Yes		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (Antigen tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Yes		

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Weitzel 2020 [A] (Continued)

If a threshold was used, was it pre-specified? Yes

Could the conduct or interpretation of the index test have introduced bias? Low risk

Are there concerns that the index test, its conduct, or interpretation differ from the review question? High

DOMAIN 2: Index Test (Rapid PCR tests)
DOMAIN 3: Reference Standard

Is the reference standards likely to correctly classify the target condition? No

Were the reference standard results interpreted without knowledge of the results of the index tests? Yes

Reference standard does not incorporate result of index test? Yes

Could the reference standard, its conduct, or its interpretation have introduced bias? High risk

Are there concerns that the target condition as defined by the reference standard does not match the question? High

DOMAIN 4: Flow and Timing

Was there an appropriate interval between index test and reference standard? Yes

Did all patients receive the same reference standard? Yes

Were all patients included in the analysis? No

Did all participants receive a reference standard? Yes

Were results presented per patient? Yes

Could the patient flow have introduced bias? High risk

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

80

Weitzel 2020 [B]

Study characteristics

Patient Sampling See [Weitzel 2020 \[A\]](#) for full study details and QUADAS entries

Patient characteristics and setting

Index tests [Weitzel 2020 \[B\]](#) entry is for test [B] in the list below; see [Weitzel 2020 \[A\]](#) for full study details and QUADAS entries

Test name:

[A] Biocredit COVID-19 Ag One Step SARS-CoV-2 Antigen Test (RapiGEN Inc., Anyang-si, Gyeonggi-do, Republic of Korea)

[B] COVID-19 Antigen Rapid Test Device StrongStep COVID-19 Antigen Test (Liming Bio-Products Co., Jiangsu, China)

[C] Huaketai New Coronavirus (SARS-CoV-2) N Protein Detection Kit (Fluorescence immunochromatography) (Savant Biotechnology Co., Beijing, China),

[D] Diagnostic Kit for 2019-Novel Coronavirus (2019-nCoV) Ag Test (Fluorescence Immunochromatographic Assay) (Bioeasy Biotechnology Co., Shenzhen, China).

Manufacturer:

[A] RapiGEN Inc., Anyang-si, Gyeonggi-do, Republic of Korea

[B] Liming Bio-Products Co., Jiangsu, China

[C] Savant Biotechnology Co., Beijing, China

[D] Bioeasy Biotechnology Co., Shenzhen, China

Antigen target: not reported in study

Antibody: not reported in study

Test method: [A] and [B] CGIA
[C] and [D] FIA

Samples used: NOP swabs in 3 mL UTM

Transport media: UTM-RT System (Copan Diagnostics, Murrieta, CA, USA)

Sample storage: stored at -80 °C; index tests applied on 28 and 29 April 2020

Test operator: single, trained laboratory technician under BSL2 cabinet; visual outputs read by 2 independent observers with referral to third if needed

Definition of test positivity: as per manufacturer; Savant test required use of manufacturer supplied UV torch due to unavailability of reader device in Chile

Blinding reported: yes; blinding stated

Timing of samples: median 2 days (IQR 1-5 days); 88% (96/109) during the first week of symptoms

Target condition and reference standard(s) See [Weitzel 2020 \[A\]](#) for full study details and QUADAS entries

Flow and timing See [Weitzel 2020 \[A\]](#) for full study details and QUADAS entries

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Weitzel 2020 [B] (Continued)

Comparative

Notes

Weitzel 2020 [C]

Study characteristics

Patient Sampling See [Weitzel 2020 \[A\]](#) for full study details and QUADAS entries

Patient characteristics and setting See [Weitzel 2020 \[A\]](#) for full study details and QUADAS entries

Index tests [Weitzel 2020 \[C\]](#) entry is for test [C] in the list below; see [Weitzel 2020 \[A\]](#) for full study details and QUADAS entries

Test name:

[A] Biocredit COVID-19 Ag One Step SARS-CoV-2 Antigen Test (RapiGEN Inc., Anyang-si, Gyeonggi-do, Republic of Korea)

[B] COVID-19 Antigen Rapid Test Device StrongStep COVID-19 Antigen Test (Liming Bio-Products Co., Jiangsu, China)

[C] Huaketai New Coronavirus (SARS-CoV-2) N Protein Detection Kit (Fluorescence immunochromatography) (Savant Biotechnology Co., Beijing, China),

[D] Diagnostic Kit for 2019-Novel Coronavirus (2019-nCoV) Ag Test (Fluorescence Immunochromatographic Assay) (Bioeasy Biotechnology Co., Shenzhen, China).

Manufacturer:

[A] RapiGEN Inc., Anyang-si, Gyeonggi-do, Republic of Korea

[B] Liming Bio-Products Co., Jiangsu, China

[C] Savant Biotechnology Co., Beijing, China

[D] Bioeasy Biotechnology Co., Shenzhen, China

Antigen target: not reported in study

Antibody: not reported in study

Test method: [A] and [B] CGIA

[C] and [D] FIA

Samples used: NOP swabs in 3 mL UTM

Transport media: UTM-RT System (Copan Diagnostics, Murrieta, CA, USA)

Sample storage: stored at -80 °C; index tests applied on 28 and 29 April 2020

Test operator: single, trained laboratory technician under BSL2 cabinet; visual outputs read by 2 independent observers with referral to third if needed

Definition of test positivity: as per manufacturer; Savant test required use of manufacturer supplied UV torch due to unavailability of reader device in Chile

Blinding reported: yes; blinding stated

Timing of samples: median 2 days (IQR 1-5 days); 88% (96/109) during the first week of symptoms

Target condition and ref- See [Weitzel 2020 \[A\]](#) for full study details and QUADAS entries

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Weitzel 2020 [C] (Continued)

erence stan-
dard(s)

Flow and tim-
ing See [Weitzel 2020 \[A\]](#) for full study details and QUADAS entries

Comparative

Notes

Weitzel 2020 [D]

Study characteristics

Patient Sam-
pling See [Weitzel 2020 \[A\]](#) for full study details and QUADAS entries

Patient char-
acteristics and
setting See [Weitzel 2020 \[A\]](#) for full study details and QUADAS entries

Index tests [Weitzel 2020 \[D\]](#) entry is for test [D] in the list below; see [Weitzel 2020 \[A\]](#) for full study details and QUADAS entries

Test name:

[A] Biocredit COVID-19 Ag One Step SARS-CoV-2 Antigen Test (RapiGEN Inc., Anyang-si, Gyeonggi-do, Republic of Korea)

[B] COVID-19 Antigen Rapid Test Device StrongStep® COVID-19 Antigen Test (Liming Bio-Products Co., Jiangsu, China)

[C] Huaketai New Coronavirus (SARS-CoV-2) N Protein Detection Kit (Fluorescence immunochromatography) (Savant Biotechnology Co., Beijing, China),

[D] Diagnostic Kit for 2019-Novel Coronavirus (2019-nCoV) Ag Test (Fluorescence Immunochromatographic Assay) (Bioeasy Biotechnology Co., Shenzhen, China).

Manufacturer:

[A] RapiGEN Inc., Anyang-si, Gyeonggi-do, Republic of Korea

[B] Liming Bio-Products Co., Jiangsu, China

[C] Savant Biotechnology Co., Beijing, China

[D] Bioeasy Biotechnology Co., Shenzhen, China

Antigen target: not reported in study

Antibody: not reported in study

Test method: [A] and [B] CGIA

[C] and [D] FIA

Samples used: NOP swabs in 3 mL UTM

Transport media: UTM-RT System (Copan Diagnostics, Murrieta, CA, USA)

Sample storage: stored at -80°C; index tests applied on 28 and 29 April 2020

Test operator: single, trained laboratory technician under BSL2 cabinet; visual outputs read by 2 independent observers with referral to third if needed

Definition of test positivity: as per manufacturer; Savant test required use of manufacturer supplied UV torch due to unavailability of reader device in Chile

Weitzel 2020 [D] (Continued)

Blinding reported: yes; blinding stated

Timing of samples: median 2 days (IQR 1-5 days); 88% (96/109) during the first week of symptoms

Target condition and reference standard(s)

See [Weitzel 2020 \[A\]](#) for full study details and QUADAS entries

Flow and timing

See [Weitzel 2020 \[A\]](#) for full study details and QUADAS entries

Comparative

Notes

Wolters 2020

Study characteristics

Patient Sampling

2-group study to estimate sensitivity and specificity for diagnosis of active disease:
- samples selected from laboratories on the basis of presence/absence of 2 genetic targets on RT-PCR: SARS-CoV-2 E-gene +/RdRp gene + (n = 30); SARS-CoV-2 E-gene +/RdRp gene - (n = 28); SARS-CoV-2 E-gene -/RdRp gene (n = 30)
(A separate set of samples were tested in triplicate at all 3 laboratories to determine limits of detection and analytical specificity)

Recruitment: not stated; deliberate sampling used

Prospective or retrospective: retrospective

Sample size (cases): 88 (58)

Patient characteristics and setting

Setting: not stated; 3 laboratories

Location: Radboud UMC in Nijmegen, PAMM in Veldhoven and the RIVM in Bilthoven

Country: The Netherlands

Dates: January-March 2020

Symptoms and severity: not stated

Demographics: not stated

Exposure history: not stated

Index tests

Test name: Cepheid Xpert Xpress SARS-CoV-2 (product code not reported)

Manufacturer: Cepheid Europe

Antigen target: E-gene (sarbeco-specific) and N2-gene (SARS-CoV-2-specific)

Antibody: N/A

Test method: not stated (it should be automated PCR)

Samples used: NP or mid-turbinate, and OP swabs

Transport media: UTM or GLY medium; no further details

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Wolters 2020 (Continued)

	<p>Sample storage: stored at -80°C</p> <p>Test operator: not stated; presume laboratory staff</p> <p>Definition of test positivity: as per manufacturer; reported E-gene-only positive specimens as pre-sumptive positive but no re-testing with Xpert Xpress was reported. N2-only positives were considered positive (but re-tested with RT-PCR)</p> <p>Blinding reported: not stated (see comment section)</p> <p>Timing of samples: not stated</p>
Target condition and reference standard(s)	<p>Reference standard: in-house RT-PCR: Radboud UMC Lab: MagNApure 96 (Roche) (isolation platform); MagNApure 96 DNA and Viral NA Small Volume (extraction kit); Roche LC480 II (PCR platform); Life Technologies Taqman FastVirus 1-step mastermix (RT-PCR mastermix) PAMM Lab: Roche cobas 4800 (isolation platform); CT/NG extraction protocol (extraction kit); Roche LC480 II (PCR platform); Roche LightCycler Multiplex RNA Virus Master (RT-PCR mastermix); RIVM Lab: BioMérieux NucliSens (isolation platform); easyMAG EasyMAG extraction reagents (extraction kit); Thermo Fisher QuantStudio 6 (PCR platform); Life Technologies Taqman FastVirus 1-step mastermix (RT-PCR mastermix)</p> <p>Definition of non-COVID cases: yes (performed prior to index test)</p> <p>Genetic target(s): Radboud UMC lab: E-gene and RdRp-gene PAMM Lab: started with E-gene and RdRp-gene and mid-March moved on to E-gene testing only RIVM Lab: started with E-gene and RdRp-gene and at the beginning of April moved on to E-gene and CDC N1-gene primer and probes</p> <p>Samples used: as for index test</p> <p>Timing of reference standard: as for index test</p> <p>Blinded to index test: storage prior to freezing was not reported; samples were analysed at or near time of collection ("processed ... in the routine diagnostic procedure using the locally implemented RT-PCR")</p> <p>Incorporated index test: no</p>
Flow and timing	<p>Time interval between index and reference tests: same samples used; index test seems to have been conducted after frozen storage</p> <p>All participants received same reference standard: no, 3 different in-house PCR based on the laboratory</p> <p>Missing data: none reported</p> <p>Uninterpretable results: none reported</p> <p>Indeterminate results (index test): 1 sample was positive only on N2 gene (positive according to IFU) and 1 was positive only on E gene (presumptive positive, requires re-testing according to IFU). Both samples were re-tested on RT-PCR only</p> <p>Indeterminate results (reference standard): re-testing of the two 'FN' samples (one TP and 1 presumptive positive according to IFU definition) with RT-PCR found both samples to be disease-negative (reclassified as 1 TN and 1 FP); study authors note that the viral loads of these samples are at the limit of detection for Xpert Xpress and that multiple freeze-thaw steps of samples could have had a significant impact on detection.</p> <p>Unit of analysis: not stated; only samples reported</p>
Comparative	
Notes	Funding: not stated

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Wolters 2020 (Continued)

Publication status: accepted manuscript

Source: Journal of Clinical Virology

Author COI: the study authors declare no COI present

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	No		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (Antigen tests)			
DOMAIN 2: Index Test (Rapid PCR tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	No		
Could the conduct or interpretation of the index test have introduced bias?		High risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Wolters 2020 (Continued)

Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes	
Reference standard does not incorporate result of index test?	Yes	
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk
Are there concerns that the target condition as defined by the reference standard does not match the question?		High
DOMAIN 4: Flow and Timing		
Was there an appropriate interval between index test and reference standard?	Yes	
Did all patients receive the same reference standard?	Yes	
Were all patients included in the analysis?	Unclear	
Did all participants receive a reference standard?	Yes	
Were results presented per patient?	Unclear	
Could the patient flow have introduced bias?		Unclear risk

Zhen 2020 [A]
Study characteristics

Patient Sampling	2-group study to estimate sensitivity and specificity: - samples from symptomatic patients of all ages and gender Recruitment: not stated; specimens selected to represent the true positivity rate at authors' institution (50% to 60%), and to span low and high viral loads Prospective or retrospective: mixed; included frozen samples (n = 88) and prospectively tested (n = 20) Number of samples (samples with confirmed SARS-CoV-2):108 (58)
Patient characteristics and setting	Setting: not stated; selected from laboratory Location: not stated; authors' institutions were Northwell Health Laboratories, and Dept Pathology and Laboratory Medicine, The Donald and Barbara Zucker School of Medicine

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Zhen 2020 [A] (Continued)

Country: USA

Dates: March-April 2020

Symptoms and severity: "symptomatic"; no further details

Demographics: not stated (all ages and genders)

Exposure history: not stated

Index tests

[Zhen 2020 \[A\]](#) is the entry for test [A] from the list below

Test name:

[A] Xpert® Xpress SARS-CoV-2

[B] ID NOW COVID-19

(no product codes reported)

Manufacturer: [A] Cepheid, [B] Abbott

Antigen target: [A] N2, E; [B] RdRp

Antibody: N/A

Test method: rapid PCR

Samples used: NP swabs

Transport media: UTM (various manufacturers)

Sample storage: on collection, stored at 2-8 °C for up to 72 h; after routine testing, stored at -80 °C

88 samples tested using ePlex on collection, then frozen prior to testing with ID NOW, Xpert Xpress and Hologic RT-PCR; 20 samples tested prospectively after collection on all systems

Test operator: not stated; presume laboratory staff

Definition of test positivity: not stated; states "testing was performed according to the manufacturer's instructions" but no presumptive positives reported

Blinding reported: not stated

Timing of samples: not stated

Study also evaluates [C] GenMar kePlex® SARS-CoV-2 Test (not eligible for this review)

Target condition and reference standard(s)

Reference standard: RT-PCR; Hologic Panther Fusion SARS-CoV-2 assay, performed according to manufacturer's IFU

Definition of non-COVID cases: single RT-PCR

Genetic target(s): 2 regions of ORF1ab; either positive

Samples used: NP swabs; same as for index test

Timing of reference standard: not stated

Blinded to index test: not stated

Incorporated index test: no

Flow and timing

Time interval between index and reference tests: not stated in exact terms; delay between index and reference only for GenMark assay, as 88 samples tested at time of collection with ePlex then frozen before testing with all other assays.

Zhen 2020 [A] (Continued)

All participants received same reference standard: yes

Missing data: none reported

Uninterpretable results: 1 specimen with invalid result on ID NOW was excluded from that dataset

Indeterminate results (index test): none reported; no re-testing conducted

Indeterminate results (reference standard): none reported; no re-testing conducted

Unit of analysis: not stated only refers to samples

Comparative

Notes

Funding: none stated; study authors thank Cepheid for providing the reagents used

Publication status: accepted manuscript

Source: Journal of Clinical Microbiology

Author COI: Gregory Berry has previously given education seminars for Abbott, Cepheid, and Hologic, Inc. and has received Honorariums

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	No		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Yes		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (Antigen tests)			
DOMAIN 2: Index Test (Rapid PCR tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		

Zhen 2020 [A] (Continued)

Could the conduct or interpretation of the index test have introduced bias?		Unclear risk
Are there concerns that the index test, its conduct, or interpretation differ from the review question?		High
DOMAIN 3: Reference Standard		
Is the reference standards likely to correctly classify the target condition?	No	
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear	
Reference standard does not incorporate result of index test?	Yes	
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk
Are there concerns that the target condition as defined by the reference standard does not match the question?		High
DOMAIN 4: Flow and Timing		
Was there an appropriate interval between index test and reference standard?	Yes	
Did all patients receive the same reference standard?	Yes	
Were all patients included in the analysis?	No	
Did all participants receive a reference standard?	Yes	
Were results presented per patient?	Unclear	
Could the patient flow have introduced bias?		High risk

Zhen 2020 [B]

Study characteristics	
Patient Sampling	See Zhen 2020 [A] for full study details and QUADAS entries

Zhen 2020 [B] (Continued)

Patient characteristics and setting See [Zhen 2020 \[A\]](#) for full study details and QUADAS entries

Index tests [Zhen 2020 \[B\]](#) is the entry for test [B] from the list below, see [Zhen 2020 \[A\]](#) for full study details and QUADAS entries

Test name:

[A] Xpert® Xpress SARS-CoV-2
[B] ID NOW**COVID-19**
(no product codes reported)

Manufacturer: [A] Cepheid, [B] Abbott

Antigen target: [A] N2, E; [B] RdRp

Antibody: N/A

Test method: rapid PCR

Samples used: NP swabs

Transport media: UTM (various manufacturers)

Sample storage: on collection, stored at 2-8 °C for up to 72 h; after routine testing, stored at -80 °C
88 samples tested using ePlex on collection, then frozen prior to testing with ID NOW, Xpert Xpress and Hologic RT-PCR; 20 samples tested prospectively after collection on all systems

Test operator: not stated; presume laboratory staff

Definition of test positivity: not stated; states “testing was performed according to the manufacturer’s instructions” but no presumptive positives reported

Blinding reported: not stated

Timing of samples: not stated

Study also evaluates [C] GenMar kePlex® SARS-CoV-2 Test (not eligible for this review)

Target condition and reference standard(s) See [Zhen 2020 \[A\]](#) for full study details and QUADAS entries

Flow and timing See [Zhen 2020 \[A\]](#) for full study details and QUADAS entries

Comparative

Notes Funding: none stated; study authors thank Cepheid for providing the reagents used

Publication status: accepted manuscript

Source: Journal of Clinical Microbiology

Author COI: Gregory Berry has previously given education seminars for Abbott, Cepheid, and Hologic, Inc. and has received Honorariums

BAL: bronchoalveolar lavage; **CDC:** Center for Disease Control; **CGIA:** colloidal gold immunoassay; **COI:** conflict of interest; **Ct:** cycle threshold; **ED:** Emergency Department; **EUA:** emergency use authorisation; **FIA:** fluorescence immunochromatographic; **FN:** false negative; **FP:** false positive; **GLY:** Glucose-Lactalbumin-Yeast; **HCW:** healthcare worker; **ICU:** intensive care unit; **IFU:** instructions

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

91

for use; **IQR**: interquartile range; **LDT**: laboratory-developed test; **N/A**: not applicable; **NAAT**: nucleic acids amplification test; **NIH**: National Institutes of Health; **NOP**: naso-oropharyngeal; **NP**: nasopharyngeal; **OP**: oropharyngeal; **PCR**: polymerase chain reaction; **PHE**: Public Health England; **qRT-PCR**: quantitative reverse transcription polymerase chain reaction; **RNA**: ribonucleic acid; **RT-PCR**: reverse transcription polymerase chain reaction; **SD**: standard deviation; **TA**: tracheal aspirate; **TN**: true negative; **TP**: true positive; **UTM**: universal transport medium; **UV**: ultraviolet; **UW**: University of Washington; **VTM**: viral transport medium;

Characteristics of excluded studies [ordered by study ID]

Study	Reason for exclusion
Ai 2020	Ineligible index test
Anahtar 2020	Ineligible index test
Arumugam 2020	Ineligible index test
Baek 2020	Ineligible index test
Barra 2020	Ineligible study design
Basu 2020	Ineligible reference standard
Behrmann 2020	Accuracy data cannot be extracted
Bordi 2020	Ineligible study design
Broughton 2020	Ineligible index test
Callahan 2020	Accuracy data cannot be extracted
Chandler-Brown 2020	Ineligible study design
Colson 2020	Inadequate sample size
Comar 2020	Ineligible reference standard
Crone 2020	Ineligible index test
Curti 2020	Ineligible study design
Ding 2020	Ineligible study design
Dohla 2020	Ineligible index test
Farfan 2020	Ineligible study design
Francis 2020	Ineligible study design
Freire-Paspuel 2020	Ineligible study design
Ganguli 2020	Ineligible population
Giamarellos-Bourboulis 2020	Ineligible study design
Gonzalez-Gonzalez 2020	Ineligible study design
Grant 2020	Ineligible index test

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Study	Reason for exclusion
Hass 2020	Ineligible target condition
Hogan 2020a	Ineligible index test
Hu 2020	Ineligible index test
Huang 2020	Ineligible index test
Jiang 2020	Ineligible index test
Joung 2020	Ineligible index test
Kalikiri 2020	Ineligible index test
Kim 2019	Ineligible study design
Konrad 2020	Ineligible study design
Kurstjens 2020	Ineligible index test
Lalli 2020	Inadequate sample size
Lamb 2020	Ineligible study design
Lee 2020	Ineligible index test
Lin 2020	Ineligible population
Lowe 2020	Ineligible index test
Lu 2020	Ineligible study design
Lu 2020a	Ineligible index test
Mahari 2020	Ineligible study design
Marzinotto 2020	Accuracy data cannot be extracted
McCormick-Baw 2020	Ineligible index test
McRae 2020	Ineligible index test
Mei 2020	Ineligible index test
Noerz 2020	Ineligible index test
Osterdahl 2020	Ineligible index test
Paden 2020	Ineligible study design
Pellanda 2020	Ineligible index test
Pfefferle 2020	Ineligible study design
Seo 2020	Accuracy data cannot be extracted

Study	Reason for exclusion
Smyrlaki 2020	Ineligible index test
St Hilaire 2020	Ineligible index test
Tan 2020	Ineligible study design
Visseaux 2020	Ineligible index test
Wang 2020	Ineligible index test
Wang 2020a	Accuracy data cannot be extracted
Wee 2020	Ineligible study design
Xue 2020	Ineligible index test
Yan 2020	Ineligible index test
Yang 2020	Ineligible index test
Yu 2020	Ineligible index test
Yu 2020a	Ineligible index test
Zamecnik 2020	Ineligible index test
Zeng 2020	Ineligible study design
Zhang 2020	Ineligible index test
Zhao 2020	Ineligible study design

DATA

Presented below are all the data for all of the tests entered into the review.

Table Tests. Data tables by test

Test	No. of studies	No. of participants
1 Antigen tests - All	8	1180
2 Antigen tests - high viral load	7	400
3 Antigen tests - low viral load	7	341
4 Molecular tests - all	15	2325
5 Molecular tests - all (before discrepant analysis)	4	1280
6 Molecular tests - all (after discrepant analysis)	4	1280

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test	No. of studies	No. of participants
7 Molecular tests - high viral load	5	151
8 Molecular tests - low viral load	5	142

Test 1. Antigen tests - All

Antigen tests - All

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	Sensitivity (95% CI)	Specificity (95% CI)
Diao 2020	141	0	67	31	0.68 [0.61, 0.74]	1.00 [0.89, 1.00]		
Lambert-Niclot 2020	47	0	47	44	0.50 [0.40, 0.60]	1.00 [0.92, 1.00]		
Mertens 2020	76	1	56	195	0.58 [0.49, 0.66]	0.99 [0.97, 1.00]		
Porte 2020	77	0	5	45	0.94 [0.86, 0.98]	1.00 [0.92, 1.00]		
Weitzel 2020 [A]	49	0	30	30	0.62 [0.50, 0.73]	1.00 [0.88, 1.00]		
Weitzel 2020 [B]	0	1	9	9	0.00 [0.00, 0.34]	0.90 [0.55, 1.00]		
Weitzel 2020 [C]	13	0	65	31	0.17 [0.09, 0.27]	1.00 [0.89, 1.00]		
Weitzel 2020 [D]	68	0	12	31	0.85 [0.75, 0.92]	1.00 [0.89, 1.00]		

Test 2. Antigen tests - high viral load

Antigen tests - high viral load

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	Sensitivity (95% CI)	Specificity (95% CI)
Diao 2020	55	0	1	0	0.98 [0.90, 1.00]	Not estimable		
Lambert-Niclot 2020	37	0	8	0	0.82 [0.68, 0.92]	Not estimable		
Mertens 2020	65	0	23	0	0.74 [0.63, 0.83]	Not estimable		
Porte 2020	52	0	0	0	1.00 [0.93, 1.00]	Not estimable		
Weitzel 2020 [A]	45	0	8	0	0.85 [0.72, 0.93]	Not estimable		
Weitzel 2020 [C]	11	0	41	0	0.21 [0.11, 0.35]	Not estimable		
Weitzel 2020 [D]	54	0	0	0	1.00 [0.93, 1.00]	Not estimable		


Test 3. Antigen tests - low viral load

Antigen tests - low viral load

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	Sensitivity (95% CI)	Specificity (95% CI)
Diao 2020	86	0	66	0	0.57 [0.48, 0.65]	Not estimable		
Lambert-Niclot 2020	10	0	39	0	0.20 [0.10, 0.34]	Not estimable		
Mertens 2020	11	0	33	0	0.25 [0.13, 0.40]	Not estimable		
Porte 2020	13	0	5	0	0.72 [0.47, 0.90]	Not estimable		
Weitzel 2020 [A]	4	0	22	0	0.15 [0.04, 0.35]	Not estimable		
Weitzel 2020 [C]	2	0	24	0	0.08 [0.01, 0.25]	Not estimable		
Weitzel 2020 [D]	14	0	12	0	0.54 [0.33, 0.73]	Not estimable		


Test 4. Molecular tests - all

Molecular tests - all

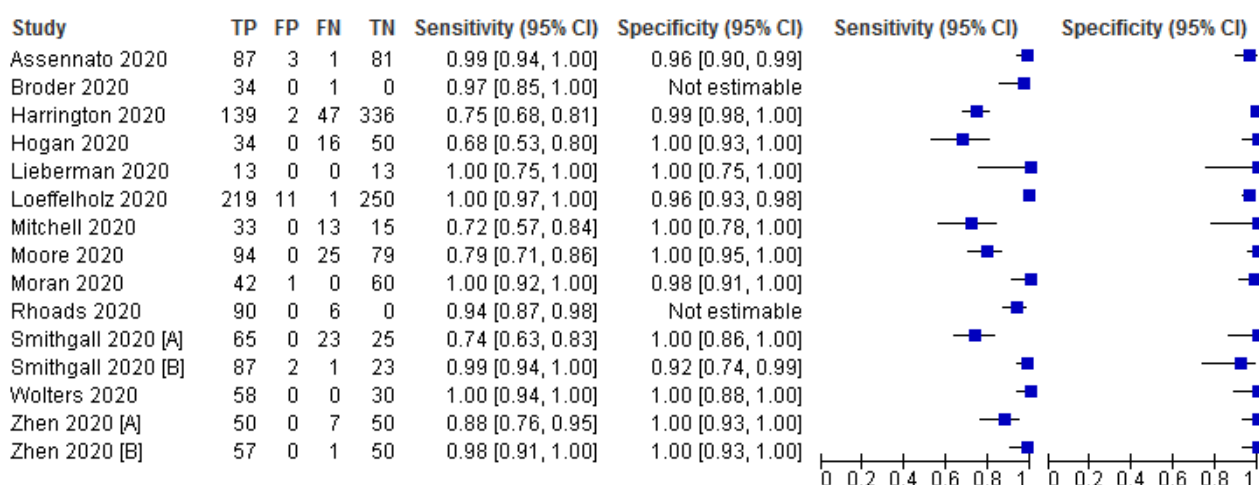


Test 5. Molecular tests - all (before discrepant analysis)

Molecular tests - all (before discrepant analysis)

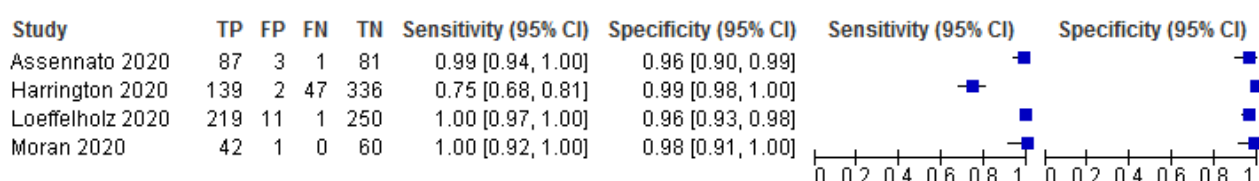


Test 6. Molecular tests - all (after discrepant analysis)

Molecular tests - all (after discrepant analysis)

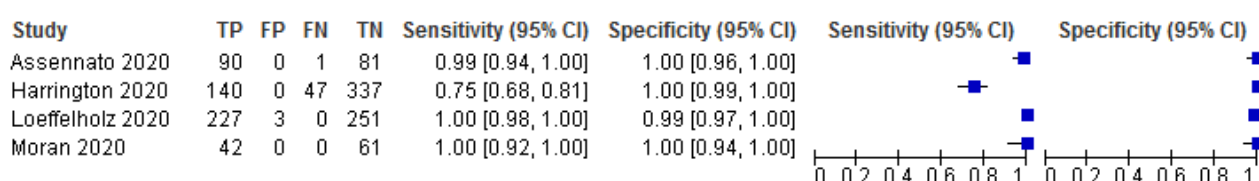


Test 7. Molecular tests - high viral load

Molecular tests - high viral load

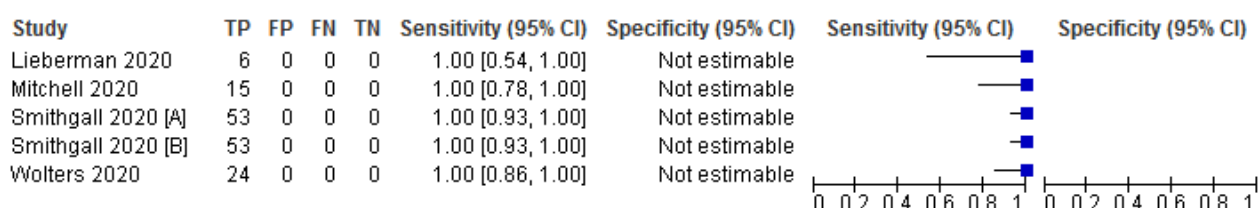

Test 8. Molecular tests - low viral load

Molecular tests - low viral load

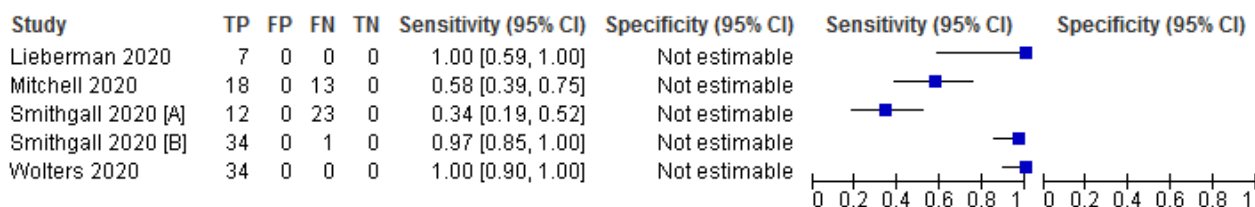

ADDITIONAL TABLES

Table 1. Description of studies

		Antigen tests	Molecular tests
Participants		5	13
Overall sample size	Median (IQR)	112 (96 to 198)	
	Range	26 to 524	
Overall number of SARS-CoV-2 positive samples	Median (IQR)	85 (50 to 119)	
	Range	13 to 220	
Sample size	Median (IQR)	138 (127 to 239)	103 (88 to 172)
	Range	111 to 328	26 to 524
Number of SARS-CoV-2 positive samples	Median (IQR)	94 (82 to 132)	58 (46 to 96)
	Range	80 to 208	13 to 220
Setting	Hospital A & E	2 (40%)	1 (8%)
	Mixed	0 (0%)	3 (31%)
	Unclear	3 (60%)	9 (69%)
Patient group	Acute (A&E presentation)	2 (40%)	1 (8%)
	Unclear	3 (60%)	12 (92%)
Study design			
Recruitment structure	Single group - sensitivity and specificity	3 (60%)	6 (46%)
	Single group - sensitivity only	0 (0)	2 (15%)

Table 1. Description of studies (Continued)

	Two or more groups - sensitivity and specificity	2 (40%)	5 (38%)
Reference standard for presence of SARS-CoV-2	All RT-PCR positive	5 (100%)	13 (100%)
Reference standard for absence of SARS-CoV-2	COVID suspects (double RT-PCR negative)	1 (20%)	0 (0%)
	COVID suspects (single RT-PCR negative)	4 (80%)	11 (85%)
	Not applicable	0 (0)	2 (15%)
Tests			
Number of tests per study	1	4 (80%)	11 (84.6%)
	2	0 (0)	2 (15.4%)
	4	1 (20%)	0 (0)
Test technology, antigen tests only ^a	Colloidal-gold immunoassay	4 (50%)	N/A
	Fluorescent immunoassay	4 (50%)	N/A
Sample type	Nasal only	0 (0%)	1 (8%)
	Nasopharyngeal only	3 (60%)	6 (46%)
	Nasopharyngeal + oropharyngeal combined	2 (40%)	1 (8%)
	Nasopharyngeal or nasal	0 (0)	3 (23%)
	Nasopharyngeal or oropharyngeal	0 (0)	1 (8%)
	Mixed (3 or more types)	0 (0)	1 (8%)
IQR: interquartile range; RT-PCR: reverse transcriptase polymerase chain reaction			

^aAs a % of antigen test evaluations (n = 8).

Table 2. Summary of analyses of test accuracy

Test	Evaluations (studies)	Samples	Cases	Average sensitivity, % (95% CI)	Average specificity, % (95% CI)
Antigen tests					
All	8 (5)	1180	762	56.2 (29.5 to 79.8)	99.5 (98.1 to 99.9)
Subgroup analysis by viral load					

Table 2. Summary of analyses of test accuracy (Continued)

High viral load	7 (5)	400	400	93.2 (63.6 to 99.1)	N/A
Low viral load	7 (5)	341	341	32.6 (17.5 to 52.6)	N/A
Difference (95% CI)				-60.6 (-83.0 to -38.2), $P < 0.001$	N/A
Subgroup analysis by test ^a					
Beijing Savant FIA	1	109	78	16.7 (9.2 to 26.8)	100 (88.8 to 100)
Coris Bioconcept CGIA ^b	2	466	226	54.4 (47.9 to 60.8)	99.6 (97.7 to 99.9)
Liming CGIA	1	19	9	0 (0 to 33.6)	90.0 (55.5 to 99.7)
RapiGEN CGIA	1	109	79	62.0 (50.4 to 72.7)	100 (88.4 to 100)
Shenzhen Bioeasy FIA ^b	2	238	162	89.5 (83.8 to 93.3)	100 (95.2 to 100)
In-house FIA	1	239	208	67.8 (61.0 to 74.1)	100 (88.8 to 100)
Subgroup analysis by sample type					
Nasopharyngeal only	3	705	434	59.4 (50.7 to 67.5)	99.6 (97.4 to 99.9)
Molecular tests					
All studies with 2x2 data	13 (11)	2194	1113	95.2 (86.7 to 98.3)	98.9 (97.3 to 99.5)
All studies ^{c,d}	15 (13)	1244	1244	95.5 (88.5 to 98.4)	N/A
Sensitivity analysis before and after discrepant analysis					
Before	4	1280	536	98.2 (87.0 to 99.8)	97.8 (94.8 to 99.1)
After	4	1280	547	99.5 (79.9 to 100)	99.6 (98.7 to 99.9)
Subgroup analyses by viral load					
High viral load ^b	5 (4)	151	151	100 (97.5 to 100)	N/A
Low viral load	5 (4)	142	142	93.3 (46.7 to 99.6)	N/A
Subgroup analyses by test ^a					
Abbott – ID NOW	5	1003	496	76.8 (72.9 to 80.3)	99.6 (98.4 to 99.9)
Cepheid – Xpert Xpress	6	919	479	99.4 (98.0 to 99.8)	96.8 (90.6 to 99.0)
Difference (95% CI)				22.6 (18.8 to 26.3), $P < 0.001$	-2.8 (-6.4 to 0.8), $P = 0.13$
Mesa Biotech – Accula	1	100	50	68.0 (53.3 to 80.5)	100 (92.9 to 100)
DRW – SAMBA II	1	172	88	98.9 (93.8 to 100)	96.4 (89.9 to 99.3)
Direct comparisons by test					

Table 2. Summary of analyses of test accuracy (Continued)

Abbott – ID NOW ^{a,b}	2	220	145	79.3 (71.8 to 85.6)	100 (95.2 to 100)
Cepheid – Xpert Xpress ^{a,b}	2	221	146	98.6 (95.1 to 99.8)	97.3 (90.7 to 99.7)
Difference (95% CI) ^e				19.3 (12.5 to 26.2), $P < 0.001$	-2.7 (-6.3 to 1.0), $P = 0.15$
Sample type					
Nasopharyngeal only ^c	6 (5)	600	343	87.1 (71.6 to 94.7)	100 (98.6 to 100)
CGIA: colloidal gold immunoassay; CI: confidence intervals; FIA: fluorescent immunoassay; DRW: Diagnostics for the Real World					

^aSee [Appendix 9](#) for details of product codes, where available (these were not necessarily reported in studies but we obtained them from manufacturer instructions for use documents).

^b2x2 tables combined prior to calculating estimates.

^cSeparate pooling of sensitivity and/or specificity.

^dThis includes two studies that only include COVID-19 positive cases.

^eTwo-sample test of proportions.

Table 3. Effect of sample re-testing

Study	Index test (target genes)	First Target RT- gene PCR	Second RT-PCR	Target gene	False positives	False negatives	Index test re-test	Reference standard re-test
Discrepant analysis								
Assennato 2020	SAMBA II (ORF1ab, N2)	PHE RdRp, E Cam-gene bridge (Wuhan) assay	PHE Col-indale RT-PCR assay	RdRp 'different region'	3 → 0	1 → 1	Yes; same results obtained	Yes; 3 FPs (reclassified as TP), all borderline positive for ≥ 1 target gene on either RT-PCR test 1 FN (remained FN), positive on both RT-PCR assays
Harrington 2020	ID NOW (RdRp)	Ab- bott Re-al-Time	Not stated	Same RT-PCR	Same	2 → 0	47 no-retest	1 FP reclassified as TN with repeat sampling 1 FP not re-tested
Loeffelholz 2020	Xpert Xpress (RUO) (E, N2)	RT-PCR varied by site: 1. New York RT-PCR assay 2. Quest 3. Al9- Re-aIS-tar 4. GeneFinder By assay 1. N (N1, N2) 2. N (N1, N3) 3. S, E 4. RdRp, E, N 5. RdRp, E, N 6. RdRp 7. RdRp, N 8. OR-PCR F1ab, S 9. OR-PCR F1ab, S 10. Re-aIS-tar 11. GeneFinder	One of: 1. Hologic Panther Fusion 2. Roche Tib-Molbiol Light-Mix 3. CDC assay	By assay: 1. ORF1ab 2. E 3. N1, N2	11 → 3	1 → 0	None reported	1 FN re-classified as TN (inconclusive positive on Quest assay; negative on CDC assay) 3 FP remained as FP (2 negative on NY assay, 1 negative on Charité Virologie assay; all confirmed negative with Hologic Panther Fusion) 8 FP re-classified as TP (all negative on Charité Virologie assay; positive on re-test with Roche Tib Molbiol assay)

Table 3. Effect of sample re-testing (Continued)

			5. See- gene Allplex						
			6. Char- ité Vi- rol- o- gy						
			7. Ab- bott Re- al- Time						
			8. Di- aSorin Sim- plexa						
Moran 2020	Xpert Xpress (E, N2)	Roch cobas 6800	ORF1, E	Same RT- PCR	Same	1 → 0	0	1 FP reclas- sified as TN (was initially E gene neg- ative and low posi- tive for N2; negative for both targets on re-test)	1 FP 'repeatedly negative' on RT-PCR re-test (re-clas- sified as TN based on index re-test)
Additional studies reporting sample re-testing (not discrepant analysis)									
Broder 2020	Xpert Xpress (E, N2)	Roch cobas 6800	ORF1a, E	modified CDC pro- tocol	NR	0	1	None re- ported No pre- sumptive positive re- sults report- ed	Yes; 1 FN (became TN)
Hogan 2020	Accula (N)	In- house SHC as- say	E gene	N/A	N/A	0	16	Yes; 1 TP re- mained as TP; faint positive Ac-	None reported

Table 3. Effect of sample re-testing (Continued)

							cula test line was repeat- ed on re-test	
Lieberman 2020	Xpert Xpress (E, N2)	CDC NI, N2 EUA- based in- house test (pos- i- tive if 1 of 2 tar- gets de- tect- ed)	N/A	N/A	0	0	Yes; 1 presump- tive positive (E-gene only positive) be- came posi- tive (N-gene only posi- tive) on re- test	None reported
Moore 2020	ID NOW (RdRp)	Mod-N1, N2 i- fied CDC RT- PCR	Abbott Re- alTime	N, RdRp	0 → 0	25 → 31	None re- ported	All samples tested with both RT-PCR assays 25 FN remained as FN (2 were inconclusive but con- sidered positive on CDC assay, confirmed positive with Abbott RealTime assay) 6 TN reclassified as FN (negative on CDC assay, con- firmed positive with Abbott RealTime assay) All 8 discordant results between the two RT-PCR's were confirmed SARS-CoV-2 positive based on record review
Wolters 2020	Xpert Xpress (E, N2)	In- By labora- house tory: as- 1. E, RdRp says at 2. E, three RdRp; lab- then E o- only ra- 3. E, to- RdRp; ries then E, N1	Same RT- PCR per laboratory	Same	0 → 2	0	None re- ported 1 presump- tive positive considered TP by review team	2 TP samples (both positive on only one target; 1 presumptive positive (E positive) and 1 positive (N2 positive)) re-classified as FP; both considered SARS- CoV-2 negative on RT-PCR re-test *authors note that viral loads were at the limit of de- tection for Xpert Xpress and that multiple freeze- thaw steps of samples could have had a significant impact on detection.

Table 3. Effect of sample re-testing *(Continued)*

CDC: center for disease control; **EUA:** emergency use authorisation; **FN:** false negative; **FP:** false positive; **PHE:** Public Health England; **RT-PCR:** reverse transcriptase polymerase chain reaction; **RUO:** research use only; **TN:** true negative; **TP:** true positive

APPENDICES

Appendix 1. Summary of World Health Organization and Chinese National Health Commission Guidelines for the diagnosis of SARS-CoV-2

Table A: World Health Organization guidelines for the diagnosis of SARS-CoV-2^a

Includes laboratory testing guidelines and global surveillance guidelines

Date range (2020)	Definition of confirmed case	Definition of confirmed non-case	Definition of suspect case	Definition of probable case	Role of serology in testing
10-30 January	10-30 January: no documentation to define at this time (before first date of global guidelines) 31 January onwards: a confirmed case is a person with laboratory confirmation of COVID-19 infection, irrespective of clinical signs and symptoms. No prescribed test in laboratory guidelines, suggested tests from 10 January include broad coronavirus RT-PCR (with sequencing of precise virus in test positives), whole genome sequencing, broad coronavirus serology on paired samples, microscopy, culture (Lab 10 January). Four suggested tests from 17 January: broad coronavirus RT-PCR (with sequencing of precise virus in test positives), NAAT for SARS-CoV-2 when it becomes available, whole genome sequencing, and broad coronavirus serology on paired samples.	None stated	No definition of 'suspect case' at this time, but case definitions for surveillance are defined as a combination of symptoms and exposure, with more severe symptoms requiring less evidence for exposure	No definition at this time	Serological testing may be useful to confirm immunologic response to a pathogen from a specific viral group, e.g. coronavirus. Best results from serologic testing requires the collection of paired serum samples (in the acute and convalescent phase) from cases under investigation.
31 January-26 February	States that once specific NAAT assays are developed and validated, confirmation will be based on specific detection of unique sequences of viral nucleic acid by RT-PCR.	None stated	Suspect case defined as combination of symptoms and exposure, with more severe symptoms requiring less evidence for exposure	A suspect case with inconclusive laboratory results or is test-positive using a pan-coronavirus assay without laboratory evidence of other respiratory pathogens (global 31 January)	
27 February-1 March		None stated	Suspect case defined as combination of symptoms and exposure, with more severe symptoms	A suspected case with inconclusive laboratory results	
2 March-19 March	A person with laboratory confirmation of COVID-19 infection, irrespective of clinical signs and symptoms (global 31 January, 27 February, 20 March)	One or more negative			In cases where NAAT assays are negative and

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

105

(Continued)

19 March-present	<p>Laboratory confirmation of cases by NAAT specific to SAR-CoV-2 such as real-time reverse-transcription polymerase chain reaction (rRT-PCR) with confirmation by nucleic acid sequencing when necessary. The viral genes targeted so far include the N, E, S and RdRP genes.</p> <p>In areas with no known COVID-19 virus circulation confirmation requires:</p> <ul style="list-style-type: none"> • NAAT positive for at least two different targets on the COVID-19 virus genome, of which at least one target is preferably specific for COVID-19 virus (or SARS-like coronavirus) using a validated assay; OR • NAAT-positive result for betacoronavirus, and COVID-19 virus identified by sequencing partial/whole genome of virus (sequence target larger or different from the amplicon probed in the NAAT assay). <p>Discordant results should be resampled.</p> <p>In areas where COVID-19 virus is widely spread a simpler algorithm might be adopted (e.g. RT-PCR of a single discriminatory target)</p>	result does not rule out the possibility of COVID-19 virus infection	toms requiring less evidence for exposure, OR defined by symptoms requiring hospitalisation and an absence of alternative explanation	(global 27 February) Probable case A suspect case for whom testing for the COVID-19 virus is inconclusive OR A suspect case for whom testing could not be performed for any reason.	there is a strong epidemiological link to COVID-19 infection, paired serum samples (in the acute and convalescent phase) could support diagnosis once validated serology tests are available. Serological assays will play an important role in research and surveillance but are not currently recommended for case detection.
------------------	--	--	---	--	--

NAAT: nucleic acids amplification test; **RT-PCR:** reverse transcription polymerase chain reaction.

^aSource data from Laboratory testing of 2019 novel coronavirus (2019-nCoV) in suspected human cases: interim guidance, World Health Organization. 10 January, 17 January, 2 March, 19 March, 21 March 2020 (WHO 2020a), and Global surveillance for COVID-19 caused by human infection with COVID-19 virus, interim guidance, 31 January, 27 February, and 20 March 2020 (WHO 2020b).

Table B: Summary of Chinese National Health Commission guidelines for diagnosis and treatment for novel coronavirus pneumonia (trial versions 1-7)

Dates in effect	Definition of confirmed case	Definition of confirmed non-case	Definition of suspect case	Role of serology in testing
16-17 January 2020 (version 1)	Cases (not confirmed cases) defined as virus genome highly homologous to coronaviruses	Not defined	Observation cases: defined as combination of exposure in Wuhan and symptoms focused on pneumonia, leukopenia and lack of improvement.	No role
18 January-2 March (versions 2, 3, 4, 5, 5 revised, and 6)	Suspect cases with either <ul style="list-style-type: none"> • real-time fluorescent RT-PCR indicates positive for new coronavirus nucleic acid; OR • viral gene sequence is highly homologous to known new coronaviruses. 	Suspect cases can be ruled out after 2 consecutive negative respiratory tract nucleic acid tests taken at least 24 hours apart.	Suspect cases: combination of exposure (such as residence in/travel to Wuhan or exposure to a confirmed case within 14 days of onset) AND clinical features (such as symptoms: fever, respiratory symptoms, and tests: chest imaging, white blood cell and lymphocyte count). Exact definition varies slightly with version	No role
3 March-present (version 7)	Suspect cases with either	Suspect cases can be ruled out after 2 negative NAATs, taken at least 24	Suspect cases: combination of exposure (such as residence in/travel to Wuhan or exposure to a confirmed case within 14 days of onset) AND clinical	Part of definition of cases and

(Continued)

- real-time fluorescent RT-PCR indicates positive for new coronavirus nucleic acid; OR
 - viral gene sequence is highly homologous to known new coronaviruses. OR
 - NCP virus-specific IgM and IgG are detectable in serum; NCP virus-specific IgG is detectable or reaches a titration of at least 4-fold increase during convalescence compared with the acute phase.
- hours apart, and the NCP virus-specific IgM and IgG are negative after 7 days from onset.
- cal features (such as symptoms: fever, respiratory symptoms, and tests: chest imaging, white blood cell and lymphocyte count).
- confirmed non-cases

NAAT: nucleic acids amplification test; **NCP:** novel coronavirus pneumonia; **RT-PCR:** reverse transcription polymerase chain reaction; Source: Table from [Cheng 2020](#)

Appendix 2. Cochrane COVID-19 Study Register searches

Source	Strategy
CT.gov	COVID-19 ^a
WHO ICTRP	Health topic: 2019-nCoV / COVID-19
PubMed	((("2019 nCoV"[tiab] OR 2019nCoV[tiab] OR "2019 novel coronavirus"[tiab] OR "COVID 19"[tiab] OR COVID19[tiab] OR "new coronavirus"[tiab] OR "novel coronavirus"[tiab] OR "novel corona virus"[tiab] OR "SARS CoV-2"[tiab] OR (Wuhan[tiab] AND (coronavirus[tiab] OR "corona virus"[tiab])) OR "COVID-19"[Supplementary Concept] OR "severe acute respiratory syndrome coronavirus 2"[Supplementary Concept]) NOT ("animals"[MeSH Terms] NOT "humans"[MeSH Terms])) NOT (editorial[pt] OR comment[pt] OR letter[pt] OR newspaper article[pt]))

^aAutomatic term mapping links results for 2019-nCoV, 2019 novel coronavirus, SARS-CoV-2, severe acute respiratory syndrome coronavirus 2.

Appendix 3. Living search from the University of Bern

The following information is taken from the university of Bern website (see: ispmbern.github.io/covid-19/living-review/collectingdata.html).

The register is updated daily and CSV file downloads are made available.

1 April 2020

From 1 April 2020, we will retrieve the curated BioRxiv/MedRxiv dataset (connect.medrxiv.org/relate/content/181).

26 to 31 March 2020

MEDLINE: ("Wuhan coronavirus" [Supplementary Concept] OR "COVID-19" OR "2019 nCoV"[tiab] OR ((("novel coronavirus"[tiab] OR "new coronavirus"[tiab]) AND (wuhan[tiab] OR 2019[tiab])) OR 2019-nCoV[All Fields] OR (wuhan[tiab] AND coronavirus[tiab])))

Embase: (nCoV or 2019-nCoV or ((new or novel or wuhan) adj3 coronavirus) or covid19 or covid-19 or SARS-CoV-2).mp.

BioRxiv/MedRxiv: nCoV or corona or wuhan or COVID or SARS-CoV-2

With the kind support of the Public Health & Primary Care Library PHC (www.unibe.ch/university/services/university_library/faculty_libraries/medicine/public_health_amp_primary_care_library_phc/index_eng.html), and following guidance of the Medical Library Association (www.mlanet.org/p/cm/ld/fid=1713).

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

1 January 2020 to 25 March 2020

MEDLINE: ("Wuhan coronavirus" [Supplementary Concept] OR "COVID-19" OR "2019 ncov"[tiab] OR (("novel coronavirus"[tiab] OR "new coronavirus"[tiab]) AND (wuhan[tiab] OR 2019[tiab])) OR 2019-nCoV[All Fields] OR (wuhan[tiab] AND coronavirus[tiab]))))

Embase: ncov OR (wuhan AND corona) OR COVID

BioRxiv/MedRxiv: ncov or corona or wuhan or COVID

Appendix 4. CDC Library, COVID-19 Research Articles Downloadable Database

Embase records from the Stephen B. Thacker CDC Library, COVID-19 Research articles Downloadable database

Records were obtained by the CDC library by searching Embase through Ovid using the following search strategy.

Source	Strategy
Embase	<p>coronavir* OR corona virus* OR betacoronavir* OR covid19 OR covid 19 OR nCoV OR novel CoV OR CoV 2 OR CoV2 OR sarscov2 OR 2019nCoV OR wuhan virus*).mp. OR ((wuhan OR hubei OR huanan) AND (severe acute respiratory OR pneumonia*) AND outbreak*).mp. OR Coronavirus infection/ OR coronavirinae/ OR exp betacoronavirus/</p> <p>Limits: 2020-</p> <p>OR</p> <p>(novel coronavir* OR novel corona virus* OR covid19 OR covid 19 OR nCoV OR novel CoV OR CoV 2 OR CoV2 OR sarscov2 OR 2019nCoV OR wuhan virus*).mp. OR ((wuhan OR hubei OR huanan) AND (severe acute respiratory OR pneumonia*) AND outbreak*).mp. OR ((wuhan OR hubei OR huanan) AND (coronavir* OR betacoronavir*)).mp.</p> <p>Limits: 2019-</p>

Appendix 5. Data extraction items

Patient sampling items	Patient characteristics and setting items	Index test items	Reference standard items	Flow and timing items	Notes items
A1 Purpose	B1 Setting	D1.1 Test name (please include product code if reported)	E1 Reference standard for cases including threshold	F1 What was the time interval between index and reference tests?	G1 Funding
A2 Design (and description of groups labelled [1] [2] ...)	B2 Location (include name of institution if available)	D1.2 Manufacturer	E1.1 RT-PCR genetic targets	F2 Did all patients receive the same reference standard?	G2 Publication status
A3 Recruitment	B3 Country	D1.3 Antigen or genetic target	E2 Samples used	F3 Missing data	G3 Source (preprint or Journal name)

(Continued)

A4 Were cases recruited prospectively or retrospectively?	B4 Dates	D1.4 Antibodies used	E3 Timing of reference standard	F4 Uninterpretable results	G4 Study author Col (including any manufacturer affiliations)
A5 Sample size (virus/COVID cases)	B5 Symptoms and severity	D1.5 POC or laboratory	E4 Was it blind to index test?	F5 Indeterminate results (index)	G5 Comment
A6 Inclusion and exclusion criteria	B6 Demographics	D1.6 Test method	E5 Did it incorporate index test?	F5.1 Indeterminate results (reference)	
A7 Comment	B7 Exposure history	D1.7 When were samples taken?	E6 Reference standard for non-cases	F6 Samples or patients	
	B8 Comment	D1.8 Samples used (include who collected by)	E7 Samples used	F7 Comment	
	Nom-COVID patients (if additional groups)	D1.8.1 Transport media (volume and manufacturer detail)	E8 Timing of reference standard		
	C1.1 Group name	D1.8.2 Sample storage and timing of test	E9 Was it blind to index test?		
	C1.2 Source and time	D1.9 Who applied the test (include reported training/e)?	E10 Did it incorporate index test?		
	C1.3 Characteristics	D1.10 How was positive defined?	E11 Comment		
	C2.1 Group name	D1.11 Blinded to reference standard			
	C2.2 Source and time	D1.12 Threshold predefined			
	C2.3 Characteristics	D1.13 Comment			

Col: conflict of interest; **POC:** point of care; **RT-PCR:** reverse transcription polymerase chain reaction

Appendix 6. Criteria for assessment of study quality (QUADAS-2)

DOMAIN: Participant selection

Was a consecutive or random sample of patients enrolled?

This will be similar for all index tests, target conditions, and populations.

Yes: if a study explicitly stated that all participants within a certain time frame were included; that this was done consecutively; or that a random selection was done.

(Continued)

	<p>No: if it was clear that a different selection procedure was employed; for example, selection based on clinician's preference, or based on institutions, or based on result of RT-PCR</p> <p>Unclear: if the selection procedure was not clear or not reported</p>
Was a case-control design avoided?	<p>This will be similar for all index tests, target conditions, and populations.</p> <p>Yes: if a study explicitly stated that all participants came from the same group of (suspected) patients.</p> <p>No: if it was clear that a different selection procedure was employed for the participants depending on their COVID-19 status or SARS-CoV-2 infection status; or if only participants with SARS-CoV-2 infection were included</p> <p>Unclear: if the selection procedure was not clear or not reported.</p>
Did the study avoid inappropriate exclusions?	<p>Studies may have excluded patients, or selected patients in such a way that they avoided including those who were difficult to diagnose or likely to be borderline. Although the inclusion and exclusion criteria will be different for the different index tests, inappropriate exclusions and inclusions will be similar for all index tests: for example, only elderly patients excluded, or children (as sampling may be more difficult). This needs to be addressed on a case-by-case basis.</p> <p>Yes: if a high proportion of eligible patients was included without clear selection.</p> <p>No: if a high proportion of eligible patients was excluded without providing a reason; if, in a retrospective study, participants without index test or reference standard results were excluded.</p> <p>Unclear: if the exclusion criteria were not reported.</p>
Did the study avoid inappropriate inclusions?	<p>Some laboratory studies may have intentionally included groups of patients in whom the accuracy was likely to differ, such as those with particularly low or high viral loads, or who had other diseases, such that the sample over-represented these groups. This needs to be addressed on a case-by-case basis.</p> <p>Yes: if samples included were likely to be representative of the spectrum of disease.</p> <p>No: if the study oversampled patients with particular characteristics likely to affect estimates of accuracy.</p> <p>Unclear: if the exclusion criteria were not reported.</p>
Could the selection of patients have introduced bias?	<p>High: if one or more signalling questions were answered with no, as any deviation from the selection process may lead to bias.</p> <p>Low: if all signalling questions were answered with yes.</p> <p>Unclear: all other instances</p>
Is there concern that the included participants do not match the review question?	<p>High: for two-group studies that included healthy or other disease controls, whether pre-pandemic or contemporaneous; studies that only included people with COVID-19 (whether RT-PCR-confirmed only, participants meeting official guideline criteria);</p> <p>Low: for single-group studies recruiting participants with signs and symptoms of COVID-19; or for two-group studies where control groups suspected of COVID-19 were separately recruited.</p> <p>Unclear: if a description about the participants was lacking.</p>
DOMAIN: Index tests	
Were the index test results interpreted without knowledge of the results of the reference standard?	<p>Yes: if blinding was explicitly stated or index test was recorded before the results from the reference standard were available.</p>

(Continued)

	<p>No: if it was explicitly stated that the index test results were interpreted with knowledge of the results of the reference standard.</p> <p>Unclear: if blinding was unclearly reported.</p>
If a threshold was used, was it prespecified?	<p>Yes: if the test was dichotomous by nature, or if the threshold was stated in the methods section, or if study authors stated that the threshold as recommended by the manufacturer was used.</p> <p>No: if a receiver operating characteristic curve was drawn or multiple threshold reported in the results section; and the final result was based on one of these thresholds.</p> <p>Unclear: if threshold selection was not clearly reported.</p>
Could the conduct or interpretation of the index test have introduced bias?	<p>High: if one or more signalling questions were answered with no, as even in a laboratory situation knowledge of the reference standard may lead to bias.</p> <p>Low: if all signalling questions were answered with yes.</p> <p>Unclear: all other instances</p>
Is there concern that the index test, its conduct, or interpretation differ from the review question?	<p>For all test types, if index test is 'in-house' or not commercially available, then state 'High'. If any test procedures used in the study diverged from IFU ((use of VTM, or testing outwith stated time limit), also state High If testing carried out in centralised laboratory and not near patient then state High. Evaluations that withheld the name of the test, or that used mixed sample types or did not report the evaluation setting, state Unclear If samples used and any sample processing steps are in accordance with test IFU, or if study describes conducting the test according to the manufacturer's protocol, state Low</p>
DOMAIN: Reference standard	
Is the reference standard likely to correctly classify the target condition?	<p>We will define acceptable reference standards using a consensus process once the list of reference standards that have been used has been obtained from the eligible studies.</p> <p>For COVID-19 cases</p> <p>Yes: RT-PCR; confirmed or suspected case using official criteria (WHO, CDC) or a clearly set out combination of signs/symptoms/exposure</p> <p>No: RT-PCR not used, or if inadequate combination of clinical characteristics used in PCR-negatives, e.g. computed tomography alone</p> <p>Unclear: if definition of COVID-19 was not reported</p> <p>For absence of COVID-19</p> <p>Yes: if at least 2 negative RT-PCR results reported if suspected COVID-19 based on signs/symptoms; single negative RT-PCR test for asymptomatic contacts or contemporaneous controls with no clinical suspicion of COVID-19; only pre-pandemic sources of control samples used.</p> <p>No: single RT-PCR or number of negative RT-PCRs not reported for COVID-19 suspects; no RT-PCR reported (untested) for asymptomatic contacts or contemporaneous controls</p> <p>Unclear: if timing of control samples (pre-pandemic or contemporaneous) was not reported</p>
Were the reference standard results interpreted without knowledge of the results of the index test?	<p>Yes: if it was explicitly stated that the reference standard results were interpreted without knowledge of the results of the index test, or if the result of the index test was obtained after the reference standard.</p> <p>No: if it was explicitly stated that the reference standard results were interpreted with knowledge of the results of the index test or if the index test was used to make the final diagnosis.</p> <p>Unclear: if blinding was unclearly reported.</p>

(Continued)

Did the definition of the reference standard incorporate results from the index test(s)?	<p>Yes: if results from the index test were a component of the reference standard definition.</p> <p>No: if the reference standard did not incorporate the index standard test.</p> <p>Unclear: if it was unclear whether the results of the index test formed part of the reference standard.</p>
Could the conduct or interpretation of the reference standard have introduced bias?	<p>High: if one or more signalling questions were answered with no.</p> <p>Low: if all signalling questions were answered with yes.</p> <p>Unclear: all other instances</p>
Is there concern that the target condition as defined by the reference standard does not match the review question?	<p>Applicability was judged primarily on the definition of disease-positive.</p> <p>High: if RT-PCR alone used to define cases</p> <p>Low: if clinical criteria, including RT-PCR, were used to define cases, regardless of whether official criteria were used, as long as the criteria were explicitly described.</p> <p>Unclear: if definition of COVID-19 cases was not provided, including if some clinically diagnosed cases were included but the clinical criteria used were not described.</p>
DOMAIN: Flow and timing	
Was there an appropriate interval between index test and reference standard?	<p>Yes: if same swab used, or swabs obtained at same time regardless of freezing (which is covered under index applicability)</p> <p>No: if different samples used with more than 24 hours between collection times</p> <p>Unclear: if can't tell</p>
Did all participants receive the same reference standard?	<p>Yes: if all participants received the same reference standard (clearly no differential verification).</p> <p>No: if (part of) the index test-positives or index test-negatives received a different reference standard.</p> <p>Unclear: if it was not reported</p>
Were all participants included in the analysis?	<p>Yes: if it is clear that all eligible participants were included in the analyses.</p> <p>No: if after the inclusion/exclusion process, participants were removed from the analyses for different reasons: no reference standard done, no index test done, intermediate results of both index test or reference standard, indeterminate results of both index test or reference standard, samples unusable.</p> <p>Unclear: if it is not possible to determine whether all participants were included (e.g. from a STARD-style participant flow diagram)</p>
Did all participants receive a reference standard?	<p>Yes: if all participants received a reference standard (clearly no partial verification).</p> <p>No: if only (part of) the index test positives or index test negatives received the complete reference standard.</p> <p>Unclear: if it was not reported</p>
Were results presented per participant?	<p>Yes: if either only one sample per participant (regardless of disaggregation of results over time), or if multiple samples per participant but results are disaggregated by time period (at least week by week)</p> <p>No: if multiple samples per participant and results are not disaggregated by time period</p>

(Continued)

Unclear: if it is not possible to tell whether results presented are per participant or per sample

Could the participant flow have introduced bias?

High: if one or more signalling questions were answered with no.

Low: if all signalling questions were answered with yes.

Unclear: all other instances

CDC: Centers for Disease Control; **ICU:** intensive care unit; **IFU:** instructions for use; **RT-PCR:** real-time polymerase chain reaction; **SARS-CoV-2:** severe acute respiratory syndrome coronavirus 2; **VTM:** viral transport medium; **WHO:** World Health Organization

Footnotes
Appendix 7. Summary study details

Study	Study design Inclusion criteria	Setting Country (Recruitment dates)	Participant characteristics	Reference standard	Reference samples and timing	Missing data Uninterpretable results Indeterminate results
Antigen tests						
Diao 2020	Single group Samples from (Preprint) cases of suspected SARS-CoV-2 infection	Not stated China (Not stated)	Not stated High viral load (≤ 30 Ct): 56, 27% (reported for 208 samples)	RT-PCR (Daan Gene kit) Threshold < 40 Ct; threshold < 30 Ct also investigated Target: ORF1ab and N gene	As for index test; NP swab Timing of reference: not stated Interval from/to index test: done in parallel	Not reported Not reported Reference: "indeterminate" category introduced into the reference standard for values between 30 and 40 Index: not reported
Lambert-Niclot 2020	Single group Samples submitted for RT-PCR testing	Not stated France (1-15 April 2020)	Not stated High viral load (≤ 25 Ct): 45, 48% (reported)	RT-PCR (different kits used) Target: E gene	As for index test; NP swab Timing of reference: within a few hours after collection Interval from/to index test: same sam-	4 samples in cobas VTM gave invalid results so all samples in cobas medium were excluded Same as above Reference: none reported

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

u-script)			ed for 94 samples)		ple, both tests conducted within a few hours	Index: control lines "barely visible" for 9 positive and 8 negative tests
138 samples						
(94 cases)						
Mertens 2020	Single group Samples from (Preprint) cases of suspected SARS-CoV-2 infection	Not stated (university laboratory)	Not reported High viral load (≤ 25 Ct): 88, 67% (reported for 132 samples)	qRT-PCR (4 different kits used) Target: 1. not stated; 2. RdRp and E genes 3. "slightly adapted" E-gene 4. E gene and ORF1-ab	As for index test; respiratory specimens (322 NP swabs, 4 NP aspirate and 2 BAL) Timing of reference: analysed at time of collection Interval from/to index test: same samples used; "some delay" between PCR and antigen testing	No None reported Reference: none reported Index: weak T lines considered positive
Porte 2020	Two groups; deliberate sampling of PCR-positive and negative cases 2:1 Samples from cohort of suspected COVID-19 cases (n = 1453); patients with respiratory symptoms and/or fever and an epidemiological risk factor for SARS-CoV-2 infection (travel or contact with case)	Out-patients at private hospital emergency room Chile (16-21 March 2020)	Cough 94 (74.6%); Fever 77 (61.1%); Median duration of symptoms 2 days (IQR 1-4; range 0-12); 68 male (53.5%); median age 38 years (IQR 29.5-44; range 1-91) High viral load (≤ 25 Ct): 52, 74% (reported for 70 samples)	RT-PCR (COVID-19 Genesig Real-Time PCR assay (Primer Design Ltd., Chander's Ford, UK)) Threshold ≤ 40 Ct Target: not stated	As for index test; OP and NP swabs Timing of reference: median 2 days post-symptom onset (IQR 1-4; range 0-12) Interval from/to index test: same sample used; within 48 hours	No Not reported Reference: patients Index: not reported
Weitzel 2020 [A]	Two groups; deliberate sampling of PCR-positive and negative cases 2:1	ED (private hospital)	Respiratory symptoms	RT-PCR (COVID-19 Genesig Real-Time PCR assay (Primerdesign Ltd., Chander's Ford, UK)) Threshold ≤ 40 Ct	As for index test; NOP swabs Timing of reference: as for index test; median 2 days (IQR 1-5)	2 invalid excluded 2 invalid results in 2 tests due to insufficient liquid migration

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

(Continued)

111 samples (80 cases)	Samples from patients with respiratory symptoms and/or fever attending a private hospital ED	Chile (16-26 March 2020)	and/or fever 50 male (45%); median age 40 years High viral load (≤ 25 Ct): 54, 68% (reported for 80 samples)	Target: RdRp gene	Interval from/to index test: same samples; index tests conducted after frozen storage	Reference: none reported Index: visual interpretation of the Savant assay (using manufacturer-supplied UV torch) was reportedly difficult under daylight conditions; manufacturer's fluorescence reader not available in Chile
------------------------	--	--------------------------	---	-------------------	---	---

Rapid molecular tests

As-sen-nato 2020 (Preprint)	Single group Samples from symptomatic individuals with suspected COVID-19 sent for routine laboratory diagnosis	Not stated; supplied by PHE UK (Not stated)	Symptomatic	RT-PCR (2 different kits used); 1. Cambridge RdRp gene (Wuhan) assay 2. PHE Colindale (Reference Laboratory) assay Target: 1. RdRp, E gene 2. RdRp "different region"	As for index; combined nose and throat swab in VTM Timing of reference: not stated Interval from/to index test: not stated; likely reference carried out for routine diagnostic testing	None reported None reported Reference: all samples tested with second RT-PCR, including 3 FP and 1 FN (see Table 3) assays Index: 3 FP and 1 FN result retested using SAMBA-II (see Table 3)
172 samples (88 cases; 91 after retesting)						
Broder 2020 (Accepted manuscript)	Single group (cases) Samples positive on RT-PCR with lower range of viral load (E target Ct ≥ 30)	Not stated (laboratory) USA (Not stated)	All lower viral load	RT-PCR (Roche cobas 6800 SARS-CoV-2 assay) Target: E gene (unclear if other genetic targets as well)	As for index test; NP swab Timing of reference: not stated (presumably on presentation) Interval from/to index test: same samples; index test within 3 days of reference	None reported None reported Reference: samples positive on reference were tested by in-house assay using modified CDC protocol Index: none reported
35 samples (35 cases)						
Harington 2020 (Accepted)	Single group Symptomatic patients, diagnostic criteria for COVID-19	EDs (n = 3) or urgent care center	Not stated	RT-PCR (Abbott RealTime SARS-CoV-2 (ACOV) assay performed on the Abbott m2000 system (Abbott Molecular Inc. Des Plaines, IL)	NP swabs (paired) Timing of reference: not reported Interval from/to index test: simultaneous swab collection	None reported None reported Reference: 2 initial FPs had repeat sampling (see Table 3)

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

(Continued)						
ed man- u- script)		tres (n = 2)		Threshold: not stated		Index: none reported
		USA		Target: not stated		
524 sam- ples		(Not stat- ed)				
(186 cases)						
Hogan 2020	Single group Samples from (Preprint) adult patients from 1 hospital and paediatric and adult sam- ples from sur- rounding hospi- tals	Not stated (clini- cal vi- rology labo- rato- ry)	Not stat- ed	RT-PCR (in-house SHC as- say) Target: E gene	As for index test; NP swab Timing of reference: not stated Interval from/to in- dex test: not stated but implies that both tests undertaken in laboratory soon after sample collection	None reported 3 invalid results were re- tested; 1 positive and 2 neg- ative Reference: none reported Index: 1 known RT-PCR-pos- itive sample that showed a faint positive test line was re-tested and again showed the same faint test line (considered positive)
Lieber- man 2020	Single group Samples submit- ted for clinical di- agnostic testing (not all samples analysed for all tests)	Not stat- ed, sam- pled from labo- ratory	Not stat- ed High vi- ral load (≤ 30 Ct): 6, 46% (report- ed for 13 samples)	RT-PCR (UW CDC EUA- based in-house test) Threshold: positive if 1 of 2 targets detected - pre- sume at <40 Ct Target: NI, N2 genes	As for index test; NP swab Timing of reference: not stated Interval from/to in- dex test: all testing conducted within 72 h	None reported; addition- al data reported compar- ing Panther Fusion with Di- aSorin Simplexa Not stated Reference: inconclusive' re- sults (i.e. 1 genetic target detected) considered pos- itive due to the high speci- ficity of all assays and limit- ed cross-reactivity seen for SARS-CoV-2 primer sets Index: same as above
169 sam- ples		(Not stat- ed)				
(87 cas- es); da- ta for Xpert Xpress avail- able for on- ly 26 sam- ples (13 cases)						
Loef- fel-	Two groups; de- liberate sam- pling to enrich	Not stated	Adults at all sites (all age	RT-PCR (8 different kits used at different sites)	As for index test	4 Xpert Xpress test results were lost permanently due to a single instrument com-

(Continued)

holz 2020	for positive specimens	USA, UK, France, Italy	groups at New York City Dept. Health and Mental Hygiene and Ni-guarda Hospital)	<ol style="list-style-type: none"> 1. New York SARS-CoV-2 Real-time RT-PCR Diagnostic Panel; 2. Quest SARS-CoV-2 rRT-PCR (Quest Diagnostics, San Juan Capistrano, US) 3. RealStar SARS-CoV-2 RT-PCR Kit 1.0 (Altona Diagnostics, Hamburg, Germany) 4. GeneFinder COVID-19 Plus RealAmp Kit (ELITechGroup, Puteaux, France) 5. Allplex 2019-nCoV Assay (Seegene, Seoul, SK) 6. Charité Virology (Berlin, Germany) (in-house) 7. Abbott RealTime SARS-CoV-2 Assay (Abbott, Des Plaines, US) 8. Simplexa COVID-19 Direct (DiaSorin, Cypress, USA) 	<p>Timing of reference: as for index test</p> <p>Interval from/to index test: same samples but index test performed after frozen storage for undefined period of time (except at University Hospital, Newark where specimens were tested in real time, within 2 h by the index test)</p>	<p>puter malfunction and 1 invalid result excluded</p> <p>1 Xpert Xpress test was invalid due to a cartridge error (inadequate sample volume)</p> <p>Reference: specimens with inconclusive results by a test, and those with discrepant results between index and the RT-PCR tests were analysed by a third RT-PCR method (see Table 3). 12 specimens (8 NPS, 4 NPS/OPS) were inconclusive and considered positive for data analysis purposes in the study. 1 NPS specimen was inconclusive by the Quest SARS-CoV-2 rRT-PCR test and negative by the Xpert test. This specimen was negative by a tie-breaker NAAT.</p> <p>Index: presumptive positive results on index test were not reanalysed by the index test, but all discrepant results were reanalysed by a third RT-PCR method</p>
<p>Target:</p> <ol style="list-style-type: none"> 1. N (N1, N2) gene 2. N (N1, N3) gene 3. S, E genes 4. RdRp, E, N genes 5. RdRp, E, N genes 6. RdRp gene 7. RdRp, N genes 8. ORF1ab, S genes <p>Tie-breaker methods (for discrepant results), included: Hologic Panther Fusion (San Diego, USA), Tib-Molbiol LightMix Modular Wuhan Coronavirus E-gene RT-PCR (Roche, Basel, Switzerland); and the CDC assay (IDT primers and probes)</p>						

Mitchell 2020	Single group	Not stated; 2 independent laboratories	Not stated	RT-PCR (2 different in-house kits used) CDC EUA and NY RT-PCR	As for index test	None reported
(Accepted manuscript)	Samples positive and negative on 1/2 SARS-CoV-2 RT-PCR assays		High viral load (≤ 30 Ct): 15, 33% (report-	Target: not stated	Timing of reference: as for index test	None reported
					Interval from/to index test: same samples but used at different times (sam-	Reference: none reported
						Index: none reported

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

61 samples (46 cases)	USA (Not stated)	ed for 46 samples)			ples used for index test stored at -80 °C)	
Moore 2020 (Preprint) 200 samples (125 cases)	Two groups; consecutive (n = 94), then deliberate sampling of all PCR-positive samples plus the next PCR-negative sample after each positive Samples from symptomatic (fever or cough or shortness of breath) adult and paediatric outpatients, ED patients, and inpatients	Mixed (outpatients, ED patients and inpatients) USA (27 March-9 April 2020)	79 (39.5%) hospitalised including 29 in ICU, 76 (38%) ambulatory care including 55 seen in a designated COVID-19 screening clinic, and 45 (23%) seen at ED; 92 male (46%); mean age 50 years (SD 17)	RT-PCR (2 different methods used in all samples) 1. modified CDC RT-PCR 2. Abbott RealTime SARS-CoV-2 RT-PCR Threshold: [1] positive result required Ct <40 for both targets; negative if neither target detected and positive amplification curve for control (RP) gene; inconclusive if only one target detected at Ct<40, and test repeated [2] amplification curves reported as detected or not detected; Target: [1]N1, N2 genes [2]N, RdRp genes	As for index test; NP swab Timing of reference: not stated Interval from/to index test: all 3 tests conducted within 72 h of sample collection	2 invalid excluded 2 results were invalid on ID Now and were not retested (excluded) Reference: discordant results on RT-PCR had record review to determine presence/absence COVID-19 infection Index: none reported
Moran 2020 (Accepted manuscript) 103 samples (42 cases)	Single group Specimens collected from inpatients and ambulatory patients at the University of Chicago	Mixed (inpatient and ambulatory); samples selected from central laboratory USA (Not stated)	Not stated	RT-PCR (Roche cobas SARS-CoV-2 assay on the cobas 6800 system (Roche Molecular Systems, Branchburg, NJ)) Target: ORF1, E genes	As for index; nasal or NP swabs Timing of reference: not stated Interval from/to index test: same sample and appear to have both been conducted soon after sample collection	None reported None reported Reference: single FP was retested on RT-PCR and found to be repeatedly negative Index: single FP was retested with index test and considered negative on both targets

(Continued)

Rhoads 2020 (Accepted manuscript) 96 samples (96 cases)	Single group (cases); Samples positive using standard of care testing	Not stated; includes self-collected and provided-collected samples USA (Not stated)	Not stated	Standard of care testing for original samples; remnant samples re-tested with modified CDC RT-PCR (using 7500 Fast instrument and using alternate RNA extraction Threshold: samples with one positive target detected considered positive instead of "inconclusive" Target: N1 and N2 genes	As for index test Timing of reference: as for index test Interval from/to index test: same samples used	None reported None reported Reference: RT-PCR detected only 1/2 targets for 2 samples (both considered positive and diagnosed as positive on original sample testing); both were negative on index test) Index: none reported
Smith-gall 2020 [A] (Published) 113 samples (88 cases)	Two groups; deliberate sampling of samples with high, medium and low Ct values on the reference standard RT-PCR Patients undergoing routine clinical testing by RT-PCR	Mixed; in-patient and ED USA (8-13 April 2020)	111 adults (range 23-101 years; mean 65 years for RT-PCR-positive and 43 years for RT-PCR-negative; 2 paediatric (age 1 day and 5 days); 61 male (54%) High viral load (≤ 30 Ct): 53, 60% (reported for 88 samples)	RT-PCR (cobas SARS-CoV-2 assay on the 6800 platform (Roche Diagnostics, Indianapolis, IN)); Threshold: not stated, all Ct values < 37 on both target genes Target: ORF1 a/b, E-gene	As for index test Timing of reference: as for index test Interval from/to index test: simultaneous; same samples used	None reported None reported Reference: none reported Index: 1 sample was a presumptive positive based on detection of E-gene target but not the N2 target
Wolters 2020 (Accepted manuscript)	Two groups; deliberate sampling according to target gene Samples selected from laboratories on the basis of E gene or	Not stated; 3 laboratories	Not stated High viral load (≤ 30 Ct): 24, 41% (report-	In-house RT-PCR (3 different kits at different laboratories) Target: 1. RadboudUMC lab: E-gene and RdRp-gene	As for index test Timing of reference: as for index test Interval from/to index test: same samples used; index text seems to have been	None reported None reported Reference: re-testing of the FN and presumptive positive samples with RT-PCR (see Table 3); Index: 1 sample was positive only on N2

(Continued)

88 samples (58 cases)	RdRp on RT-PCR (n = 88)	The Netherlands (January-March 2020)	ed for 58 samples)	2. PAMM Lab: started with E-gene and RdRp-gene and in mid-March moved on to E-gene testing only 3. RIVM Lab: started with E-gene and RdRp-gene and at the beginning of April moved on to E-gene and CDC N1-gene primer and probes	conducted after frozen storage	gene (considered negative according to IFU) and one was positive only on E gene (considered presumptive positive, requiring re-testing according to IFU). Both samples were re-tested on RT-PCR only
Zhen 2020 [A] (Accepted manuscript)	Two groups; deliberate sampling to represent the true positivity rate at study authors' institution (50%-60%), and to span low and high viral loads	Not stated; selected from laboratory	Symptomatic; all ages and gender	RT-PCR (Hologic Panther Fusion SARS-CoV-2 assay) Target: 2 regions of ORF1ab; either positive	As for index; NP swabs Timing of reference: not stated Interval from/to index test: not stated in exact terms; delay between index and reference only for GenMark assay, as 88 samples tested at time of collection with ePlex then frozen before testing with all other assays	1 invalid excluded 1 specimen with invalid result on ID Now excluded from that dataset Reference: none reported; no re-testing conducted Index: none reported; no re-testing conducted
108 samples (58 cases)	Samples from symptomatic patients of all ages and gender	(March-April 2020)				

BAL: bronchoalveolar lavage; **CDC:** Centers for Disease Control; **Ct:** cycle threshold; **ED:** emergency department; **EUA:** emergency use authorisation; **FN:** false negative; **FP:** false positive; **ICU:** intensive care unit; **IFU:** instructions for use; **IQR:** interquartile range; **NAAT:** nucleic acids amplification test; **NOP:** naso-oropharyngeal; **NP:** nasopharyngeal; **OP:** oropharyngeal; **PHE:** Public Health England; **qRT-PCR:** quantitative reverse transcription polymerase chain reaction; **RT-PCR:** reverse transcription polymerase chain reaction; **UV:** ultraviolet; **UW:** University of Washington; **VTM:** viral transport medium

Appendix 8. Summary index test details

Study	Index test (manufacturer)	Test method Target	Sample details	Test operator Test threshold
Antigen tests				
Diao 2020	Not stated (in-house; co-author affiliated to Bioeasy)	FIA Nucleo-capsid protein (N-anti-gen)	Samples tested: NP in saline Timing of sampling: not stated Timing of test: not reported Storage: not reported	Not stated; presumably lab staff Threshold: mean value of the fluorescence signal plus 5 SD
Lambert-Niclot 2020	COVID-19 Ag Respi-Strip CORIS (BioConcept, Gembloux, Belgium) Product code NR	CGIA SARS-CoV-2 NP	Samples tested: NP in VTM Timing of sampling: not stated	Not stated; presumably lab staff Threshold: as per manufacturer

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

			Timing of test: not stated (soon after collection)	
			Storage: none; no cooling or freezing step used	
Mertens 2020	COVID-19 Ag Respi-Strip (Coris BioConcept (Belgium)) Product code NR	CGIA SARS-CoV and SARS-CoV-2 highly conserved nucleoprotein	Samples tested: NP in VTM Timing of sampling: not stated Timing of test: not described Storage: not reported	Laboratory technician Threshold: visible reddish-purple band appearing at the Test line position (T)
Porte 2020	Diagnostic Kit for 2019-Novel Coronavirus (2019-nCoV) Ag Test (Bioeasy Biotechnology Co., Shenzhen, China) Catalogue no.YRLF04401025, lot no. 2002N408	CGIA SARS-CoV-2 nucleocapsid protein	Samples tested: NP + OP in VTM Timing of sampling: not stated Timing of test: not described Storage: not reported	Laboratory technician Threshold: as per manufacturer
Weitzel 2020 [A]	[A] Biocredit COVID-19 Ag One Step SARS-CoV-2 Antigen Test (RapiGEN Inc., Anyang-si, Gyeonggi-do, Republic of Korea) Catalogue no. G61RHA20; Lot No. H073001SD	CGIA Not reported in study	Samples tested: NP + OP in VTM Timing of sampling: not stated Timing of test: not described Storage: not reported	Single trained laboratory technician under BSL2 cabinet; visual outputs read by 2 independent observers with referral to third if needed Threshold: as per manufacturer
Weitzel 2020 [B]	[B] COVID-19 Antigen Rapid Test Device StrongStep COVID-19 Antigen Test (Liming Bio-Products Co., Jiangsu, China) Catalogue no. 500200; Lot No. 2003014	CGIA Not reported in study		As above
Weitzel 2020 [C]	[C] Huaketai New Coronavirus (SARS-CoV-2) N Protein Detection Kit (fluorescence immunochromatography) (Savant Biotechnology Co., Beijing, China) Catalogue no. BCT-HKT-050; Lot No. 20031501	FIA N protein		As above plus test required use of manufacturer supplied UV torch due to unavailability of reader device in Chile
Weitzel 2020 [D]	[D] Diagnostic Kit for 2019-Novel Coronavirus (2019-nCoV) Ag Test (Bioeasy Biotechnology Co., Shenzhen, China). Catalogue no. YRLF04401025; Lot No. 2002N408	FIA N protein		As above

Rapid molecular tests

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

Assennato 2020	SAMBA II SARS-CoV-2 Test (Diagnostics for the Real World) Product code not reported	Isothermal PCR ORF1ab, N2 genes	Samples tested: NP + OP in VTM Timing of sampling: not stated Timing of test: not stated Storage: not stated	Not stated; presumably laboratory staff Threshold: as per manufacturer; either target present
Broder 2020	GeneXpert Xpress SARS-CoV-2 assay (Cepheid Inc) Product code not reported	RT-PCR Not stated (E gene)	Samples tested: NP Timing of sampling: not stated Timing of test: within 3 days of RT-PCR Storage: not stated	Not stated; presumably lab staff Threshold: as per manufacturer
Harrington 2020	ID Now COVID-19 assay (Abbott Laboratories) Product code not reported	Isothermal PCR Not stated	Samples tested: NP (no VTM) Timing of sampling: not stated Timing of test: not stated (soon after collection) Storage: none	On-site medical personnel (urgent care centres); laboratory personnel at each separate location (EDs) - 2 sites reportedly experienced users of ID Now (one ED and 1 urgent care centre) and 3 sites received training Threshold: as per manufacturer
Hogan 2020	Accula SARS-CoV-2 POCT (Mesa Biotech, Inc., San Diego, CA) Product code not reported	RT-PCR N gene	Samples tested: NP in VTM or saline Timing of sampling: not stated Timing of test: not stated (possibly soon after collection) Storage: not stated	Not stated; performed at the SHC Clinical Virology Laboratory Threshold: as per manufacturer
Lieberman 2020 [A]	[A] Xpert Xpress (Cepheid) Study also evaluate 4 additional tests not eligible for this review Product code not reported	RT-PCR [A] E, N2 genes	Samples tested: NP in VTM Timing of sampling: not stated Timing of test: < 72 h Storage: 4 °C with no freeze-thaws	Not stated; presumably lab staff Threshold: any 1 of 2 targets detected was considered positive for all assays; Xpert Xpress data extracted as per IFU definition (positive = both targets or N gene positive)
Loeffelholz 2020	Cepheid Xpert Xpress SARS-CoV-2 (RUO version) (Cepheid Europe) Product code not reported	RT-PCR Nucleocapsid gene (N2) and the envelope gene (E) (also detects RdRp but this does not con-	Samples tested: mixed Timing of sampling: not stated Timing of test: not stated; except 1 site < 2 h (n = 21) Storage: stored at -80 °C; except 1 site tested in real time (n = 21)	Not stated; presumably lab staff Threshold: as per manufacturer (if both targets are detected, or, if only N2 is detected, the test reports a positive result. If only the E target is detected the test reports a presumptive positive result because this target is shared among some members of the sarbecovirus subgenus of coronaviruses)

(Continued)

		tribute to positivity)		
Mitchell 2020	ID NOW COVID-19 (Abbott, Chicago, USA) Product code not reported	Isothermal PCR Not stated	Samples tested: NP in VTM Timing of sampling: not stated Timing of test: not stated Storage: stored at -80 °C	Certified laboratory personnel Threshold: as per manufacturer
Moore 2020	ID NOW (Abbott Laboratories) Product code not reported	Isothermal PCR RdRp gene	Samples tested: NP in VTM Timing of sampling: not stated Timing of test: < 72 h from collection Storage: none, or stored at 4 °C (if testing could not be completed on the same day)	Not stated; presumably lab staff Threshold: as per manufacturer
Moran 2020	Xpert Xpress SARS-CoV-2 assay (Cepheid, Sunnyvale, CA) Product code not reported	RT-PCR E, N (N2 region) genes	Samples tested: NP or nasal Timing of sampling: not stated Timing of test: not stated Storage: not stated	Not stated; presumably lab staff Threshold: as per manufacturer
Rhoads 2020	[A] ID Now (Abbott; Chicago, USA) Product code not reported Also evaluates [B] Simplexa (Diasorin; Saluggia, Italy); not eligible for this review	Isothermal PCR Not stated	Samples tested: NP in VTM or nasal in saline Timing of sampling: not stated Timing of test: not stated Storage: not stated	Not stated; presumably lab staff Threshold: as per manufacturer
Smithgall 2020 [A]	[A] ID Now (Abbott) Product code not reported	Isothermal PCR [A] RdRp gene	Samples tested: NP in VTM or nasal in saline Timing of sampling: not stated Timing of test: within 48 h collection	Not stated; presumably lab staff Threshold: as per manufacturer
Smithgall 2020 [B]	[B] Xpert Xpress (Cepheid) Product code not reported	RT-PCR [B] N2, E genes	Storage: stored at 4 °C	
Wolters 2020	Xpert Xpress SARS-CoV-2 (Cepheid Europe) Product code not reported	RT-PCR E-gene (sarbeco-specific) and N2-gene (SARS-CoV-2-specific)	Samples tested: NP or OP in VTM or GLY Timing of sampling: not stated Timing of test: not stated Storage: stored at -80 °C	Not stated; presumably lab staff Threshold: as per manufacturer: E-gene only positive specimens considered 'SARS-CoV-2 presumptive positive' and require retesting, N2 only positives deemed positive
Zhen 2020 [A]	[A] Xpert Xpress SARS-CoV-2 (Cepheid)	RT-PCR	Samples tested: NP in VTM	Not stated; presumably lab staff

(Continued)

	Product code not reported	[A] N2, E genes	Timing of sampling: not stated	Threshold: as per manufacturer
			Timing of test: for routine testing up to 72 h; 20 samples tested prospectively after collection on all systems	
Zhen 2020 [B]	[B] ID NOW COVID-19 (Abbott)	Isothermal PCR		
	Product code not reported			
	Also evaluates	[B] RdRp gene	Storage: for routine testing (ePlex) stored at 2-8 °C; then stored at -80 °C (ID Now, Xpert Xpress and Hologic RT-PCR); 20 samples tested prospectively after collection on all systems	
	[C] ePlex SARS-CoV-2 Test (GenMark); not eligible for this review			

CGIA: colloidal gold immunoassay; **ED:** emergency department; **EUA:** Emergency Use Authorisation; **FIA:** fluorescent immunoassay; **GLY:** gelatin-lactalbumin-yeast; **IFU:** instructions for use; **NP:** nasopharyngeal; **OP:** oropharyngeal; **PCR:** polymerase chain reaction; **RT-PCR:** reverse transcription polymerase chain reaction; **SD:** standard deviation; **UV:** ultraviolet; **VTM:** viral transport medium

Appendix 9. Index test details from manufacturer instructions for use documents

Index test ^a	Type of assay	Equipment	Sample types	Transport medium	Sample storage	Test interpretation
	Throughput	Kit storage				
	Time to result					
Antigen tests						
SARS-CoV-2 Antigen Fluorescence Rapid Detection Kit (Beijing Savant)	IFU not obtained	IFU not obtained	IFU not obtained	IFU not obtained	IFU not obtained	IFU not obtained
IFU: not obtained; no mention of any COVID tests on website						
COVID-19 Ag Respi-Strip (Coris BioConcept)	CGIA (paper strip method)	Paper strips in a bottle with desiccant; LY-S dilution buffer (3.5 mL or 15 mL; tubes and stoppers);	NPs or culture extract	A gel or a sponge matrix can be used	ASAP, any delay may result in a low signal intensity. If not, store frozen at -20 °C	Visual; read through collection tube.
IFU: 5723/TB/V03	Single test	4 to 30 °C	solution; samples must be liquid			Control line only (negative), T line (with or without control (positive), no control line (invalid)
	15 min					

(Continued)

COVID-19 Anti-gen Rapid Test Device (StrongStep®) (Liming Bio-Products Co., Ltd)	CGIA Single test 15 min	Test device, extraction buffer vial, extraction tubes, workstation for holding tubes 2-30°C	NP or OP	Not mentioned in IFU	ASAP; can be held in clean, dry plastic tube or sleeve up to 72 h at 15-30 °C, or 2-8 °C before processing	Visual; 2 coloured bands for positive; control band only for negative; test line only is invalid
IFU: obtained via Weitzel 2020 [A] ; REF 500200 v1						
BIOCREDIT COVID-19 Ag (RapiGEN Inc)	CGIA Single test 5-8 min	Test device, assay diluent tube and filter cap, swab for NP collection; 1-40 °C	NP swab	Not mentioned in IFU	Test ASAP after collection; if storage required then 2-8 °C for up to 12 h, or -20 °C for up to 24 h	Visual; control line only (negative), control and test lines (positive), no control line (invalid)
BIOEASY 2019-nCoV Ag Fluorescence Rapid Test Kit (Time-Resolved Fluorescence) (Shenzhen Bioeasy Biotechnology Co, Ltd)	FIA Single test 10 min	Test card, extraction solution, extraction tube, dripper, swab and ID chip. Test runs on immunofluorescence analyser (supplied separately), transfer pipette also required	Nasal swabs, throat swabs and deep sputum samples	Not mentioned in IFU	ASAP after collection, or store at 2-8 °C for ≤ 24 h; or store at -70 °C for longer periods. Avoid repeated freezing and thawing (no more than 3 times).	Automatic; positive if both detection line and control line detect a fluorescent signal, and the detection line detection value is ≥ 0.005 ng/mL; negative if fluorescent signal on control line only; invalid if no fluorescent signal, or signal only on test line
IFU: TS-IU-F027-A2 (YRLF04401025/YRLF04401050/YRLF04401100)						

Rapid molecular tests^a

ID NOW COVID-19 (Abbott Diagnostics Scarborough Inc)	Isothermal nucleic acid amplification	Sample receiver (with elution/lysis buffer), test base (with 2 sealed reaction tubes, each containing a lyophilised pellet), transfer cartridge for transfer of the eluted sample to the test base, positive and negative control swabs; requires ID NOW Instrument	Throat, nasal, NP and OP swabs (direct testing or in listed VTM)	Early versions of IFU documents multiple options but now not recommended (ID NOW COVID-19 Product	ASAP after collection, otherwise hold in original package at room temperature (15-30 °C) for up to 2 h. If longer then store at 2-8 °C for up to 24 h from collection. No mention of frozen storage	Automatic; results displayed on the instrument screen as positive, negative or presence or absence of COVID-19 Viral RNAs cannot be determined
IFU: IN190000 v1	1 cartridge per run 5-13 min					

(Continued)

Insert,
IN190000
Rev.3
2020/04:6-8)

Xpert Xpress SARS-CoV-2 test (Cepheid) IFU: XPRSARS-COV2-10	Automated RT-PCR 1-80 cartridges according to GeneXpert system used 45 min	Single-use disposable cartridges that hold the RT-PCR reagents and host the RT-PCR process, transfer pipette; run on GeneExpert System	NP swab in VTM	Swab stored in viral transport tube containing 3 mL transport medium	Store at room temperature (15–30 °C) for up to 8 h or refrigerate (2–8 °C) up to 7 days until testing performed	Automatic; displayed positive (N2+ and E+, or N2+ only), presumptive positive (E+ only), negative (both negative), no result (repeat test), instrument error
Accula SARS-Cov-2 Test (Mesa Biotech Inc.) IFU: LBL-60058 Rev A (COV4100)	RT-PCR + LFA 1 cartridge per run 30 min	Each test kit contains: test cassette, SARS-CoV-2 buffer (5.0 mL), single-use fixed volume pipette, positive + negative control swabs; Accula or Silaris dock required to run test	Throat swab and nasal swab per test; direct testing only * check this - Hogan 2020 reports use of NP swabs only	Not recommended and will invalidate the test	Prepared sample (in buffer vial) may be stored at room temperature for up to 24 h or refrigerated (2–8 °C) and tested within 72 h of sample collection. Sample may be stored for up to 1 week at –20 °C	Visually interpretation (shown as blue test and control lines on exterior of test cassette): positive (any test line at T position, with or without control line C, but with no negative control line), negative (control line only with no negative control line), invalid (appearance of negative control line or all lines absent)
SAMBA II COVID-19 Test (Diagnostics for the Real World Ltd) IFU: REF 8500-12	Isothermal PCR Single test per run 1.5 h	Each test set contains 4 cartridges for extraction, amplification and detection of the amplification products, 2 mL SCoV buffer, fixed volume pipette, 300 µL + pipette tips or transfer pipettes 300 µL, sample collection tube and sample card; SAMBA II Assay Module and Tablet module both required to run the test;	Combined nose and throat swabs, NP/OP swabs	Direct testing or UTM/VTM can be used; no limitations on type of VTM record-	Store at 2–30 °C for up to 18 h prior to testing. Freezing of samples should be avoided	Automatic; presented and stored on the connected tablet - Tablet module result: negative, positive, invalid, halted, read failure or no results; Visual reading of test strip: internal control line only (Negative), ≥ 1 of 2 test lines (ORF and/or N lines) with or without internal control line (positive), no lines (invalid); other

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

126

(Continued)

2-37°C

ed in
IFU

combinations possible in rare
cases

ASAP: as soon as possible; **CGIA:** colloidal gold immunoassay; **IFU:** instructions for use; **NP:** nasopharyngeal; **NPS:** nasopharyngeal swab; **OP:** oropharyngeal; **RNA:** ribonucleic acid; **RT-PCR:** reverse transcription polymerase chain reaction; **UVM:** universal transfer medium; **VTM:** viral transport medium

^aThe reported product codes are as reported in the instructions for use documents and may diverge from those evaluated in the included studies (product codes were reported in only two of 18 studies).

Appendix 10. Study-level assessments of study quality

Figure 8

Figure 8. Risk of bias and applicability concerns summary: review authors' judgements about each domain for each included study

	Risk of Bias					Applicability Concerns			
	Patient Selection	Index Test: Antigen tests	Index Test: Rapid PCR tests	Reference Standard	Flow and Timing	Patient Selection	Index Test: Antigen tests	Index Test: Rapid PCR tests	Reference Standard
Assennato 2020	?		+	-	?	?		?	-
Broder 2020	-		?	?	?	-		?	-
Diao 2020	?	?		+	?	?	-		-
Harrington 2020	+		+	-	+	+		-	-
Hogan 2020	?		?	-	?	-		-	-
Lambert-Niclot 2020	?	?		-	-	?	?		-
Lieberman 2020	?		?	-	?	-		?	-
Loeffelholz 2020	-		?	-	-	-		-	-
Mertens 2020	+	?		-	+	-	-		-
Mitchell 2020	?		?	-	?	-		-	-
Moore 2020	-		?	?	-	-		-	+
Moran 2020	?		-	?	?	?		?	-
Porte 2020	-	+		-	+	-	-		-
Rhoads 2020	-		?	?	?	-		-	-
Smithgall 2020 [A]	-		-	-	?	-		-	-
Weitzel 2020 [A]	-	+		-	-	-	-		-
Wolters 2020	-		-	-	?	-		-	-
Zhen 2020 [A]	-		?	-	-	-		-	-

High
Unclear
Low

Appendix 11. Planned heterogeneity investigations

Test subgroups	Number of studies (test evaluations)	Number of COVID-19 cases	Number of non COVID-19 cases
Study design			
Antigen tests			
Single group – sensitivity and specificity	3 (3)	434	271
Two or more groups – sensitivity and specificity	5 (2)	328	147
Rapid molecular tests			
Single group – sensitivity and specificity	6 (6)	425	561
Two or more groups – sensitivity and specificity	5 (7)	688	520
Sample type			
Antigen tests			
NP only	3 (3)	434	271
NP+OP	5 (2)	328	147
Mixed (3 or more types)	0 (0)	n/a	n/a
Rapid molecular tests			
NP only	6 (7)	529	595
NP+OP	1 (1)	88	84
Mixed (3 or more types)	4 (5)	496	402
NP: nasopharyngeal; OP: oropharyngeal			

HISTORY

Review first published: Issue 8, 2020

CONTRIBUTIONS OF AUTHORS

JJD was the contact person with the editorial base.

JDi co-ordinated contributions from the co-authors and wrote the final draft of the review.

JJD, JDi, YT, CD, STP, IH, AA, LFR, MP, JDr, SB screened papers against eligibility criteria.

RS conducted the literature searches.

JDi and AA appraised the quality of papers.

JDi and AA extracted data for the review and sought additional information about papers.

JDi entered data into [Review Manager 2014](#).

JDi, JJD and SB, analysed and interpreted data.

JJD, JDi, YT, CD, STP, RS, ML, LH, AVB, DE, SD, JC worked on the methods sections and commented on the draft review.

JJD and JDi responded to the comments of the referees.

Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection (Review)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

JJD is the guarantor of the update.

DECLARATIONS OF INTEREST

Jonathan J Deeks: none known

Jacqueline Dinnes: none known

Yemisi Takwoingi: none known

Clare Davenport: none known

Mariska MG Leeflang: none known

René Spijker: the Dutch Cochrane Centre (DCC) has received grants for performing commissioned systematic reviews. In no situation, the commissioner had any influence on the results of the work.

Lotty Hooft: none known

Ann Van den Bruel: none known

Devy Emperador: is employed by FIND with funding from DFID and KFW. FIND is a global non-for profit product development partnership and WHO Diagnostic Collaboration Centre. It is FIND's role to accelerate access to high quality diagnostic tools for low resource settings and this is achieved by supporting both R&D and access activities for a wide range of diseases, including COVID-19. FIND has several clinical research projects to evaluate multiple new diagnostic tests against published Target Product Profiles that have been defined through consensus processes. These studies are for diagnostic products developed by private sector companies who provide access to know-how, equipment/reagents, and contribute through unrestricted donations as per FIND policy and external SAC review.

Sabine Dittrich: is employed by FIND with funding from DFID and Australian Aid. FIND is a global non-for profit product development partnership and WHO Diagnostic Collaboration Centre. It is FIND's role to accelerate access to high quality diagnostic tools for low resource settings and this is achieved by supporting both R&D and access activities for a wide range of diseases, including COVID-19. FIND has several clinical research projects to evaluate multiple new diagnostic tests against published Target Product Profiles that have been defined through consensus processes. These studies are for diagnostic products developed by private sector companies who provide access to know-how, equipment/reagents, and contribute through unrestricted donations as per FIND policy and external SAC review.

Ada Adriano: none known

Sophie Beese: none known

Janine Dretzke: none known

Lavinia Ferrante di Ruffano: none known

Isobel Harris: none known

Malcolm Price: none known

Sian Taylor-Phillips: none known

Sarah Berhane: is funded by NIHR Birmingham Biomedical Research Centre.

Jane Cunningham: none known

SOURCES OF SUPPORT

Internal sources

- Liverpool School of Tropical Medicine, UK
- University of Birmingham, UK

External sources

- Department for International Development, UK
Project number: 300342-104
- National Institute for Health Research (NIHR), UK

- NIHR Birmingham Biomedical Research Centre at the University Hospitals Birmingham NHS Foundation Trust and the University of Birmingham, UK

DIFFERENCES BETWEEN PROTOCOL AND REVIEW

We planned to check the following websites for eligible index tests, however these did not prove to be very accessible or easy to use and, after initial review, were not further considered:

- National Institute for Health Research (NIHR) Innovation Observatory (www.io.nihr.ac.uk/)
- www.rapidmicrobiology.com/test-method/testing-for-the-wuhan-coronavirus-a-k-a-covid-19-sars-cov-2-and-2019-ncov

We planned to check the following evidence repository for additional eligible studies however, the EPPI-Centre and Norwegian Institute of Public Health resources proved to be more accessible therefore we decided to prioritise our other sources of evidence.

- Meta-evidence (meta-evidence.co.uk/the-role-of-evidence-synthesis-in-covid19/)

We intended for two authors to independently perform data extraction, however one review author extracted study characteristics, and a second author checked them. Contingency table data were extracted independently by two review authors as planned.

We planned to evaluate the effect of additional sources of heterogeneity, including study design, reference standard, length and severity of symptoms, and setting. However, additional formal investigations using meta-regression were not possible because of limited data, lack of reporting or lack of variability across the studies in these features.

We planned to conduct a sensitivity analysis excluding studies that are solely published as preprints. We have inadequate study numbers to allow this at present but will reconsider for the next update.

INDEX TERMS

Medical Subject Headings (MeSH)

Antigens, Viral [analysis]; *Betacoronavirus; Clinical Laboratory Techniques [*methods]; Coronavirus Infections [*diagnosis] [epidemiology]; False Negative Reactions; False Positive Reactions; Pandemics; Pneumonia, Viral [*diagnosis] [epidemiology]; *Point-of-Care Systems; Sensitivity and Specificity

MeSH check words

Humans